

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018525.D
 Acq On : 01 Feb 2022 22:11
 Operator : CG/JU
 Sample : PB142349BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349

Quant Time: Feb 02 04:46:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	415	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1482	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	856	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.294	188	1645	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.468	240	1289	0.400	ng/ul	# 0.00
23) Perylene-d12	23.861	264	1392	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	3264	6.828	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	837	0.419	ng/ul	0.00
18) Fluoranthene-d10	19.319	212	1820	0.505	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.947	266	129	0.882	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018525.D
Acq On : 01 Feb 2022 22:11
Operator : CG/JU
Sample : PB142349BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349


Quant Time: Feb 02 04:46:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration

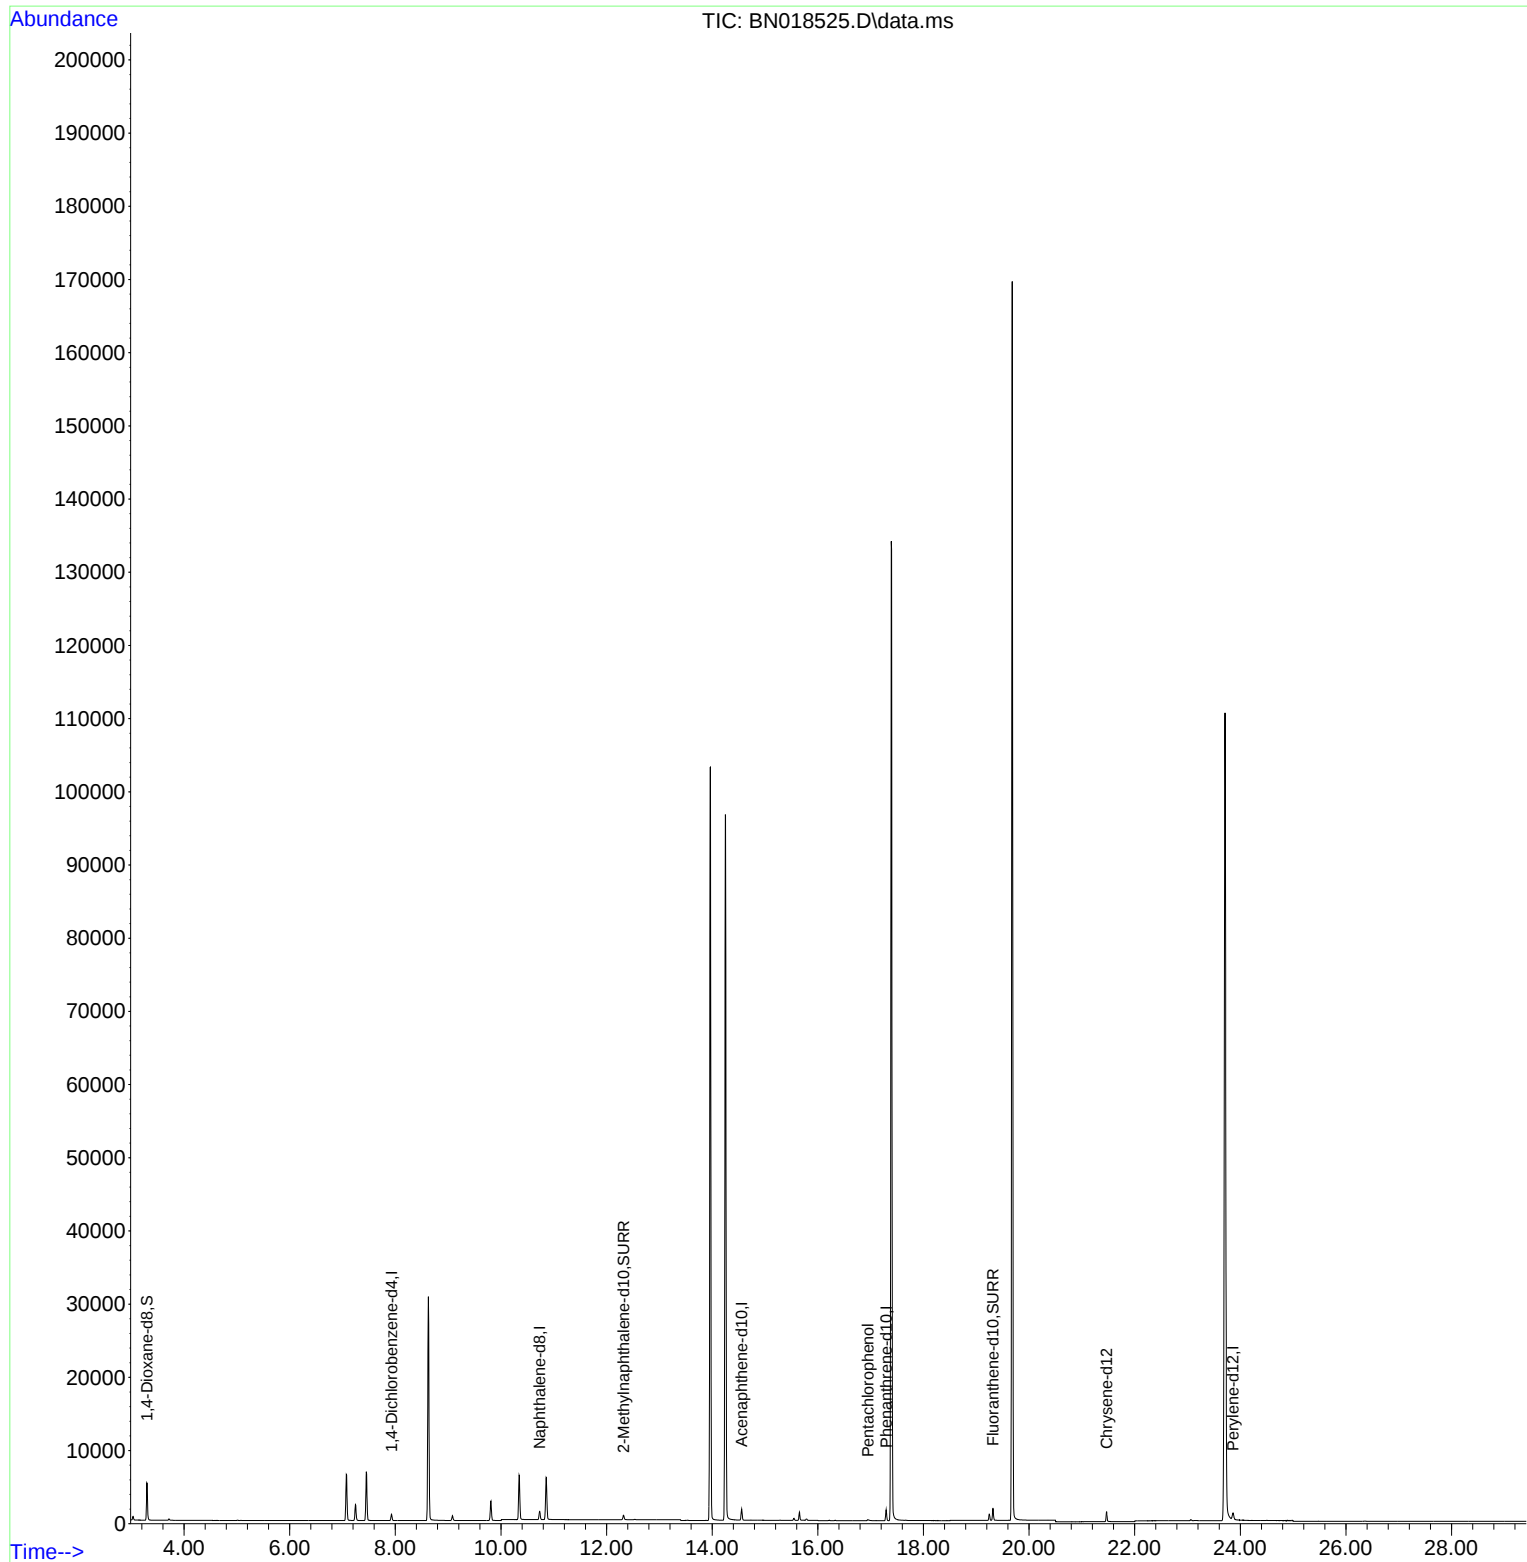

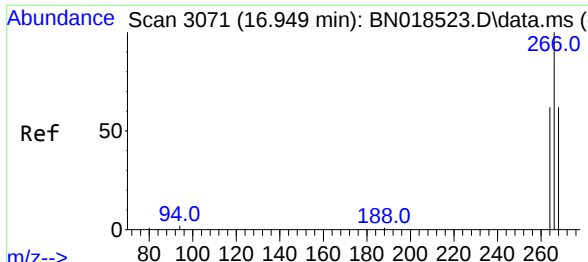

#14
 Pentachlorophenol
 Concen: 0.882 ng/ul
 RT: 16.947 min Scan# 30
 Delta R.T. -0.001 min
 Lab File: BN018525.D
 Acq: 01 Feb 2022 22:11

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349

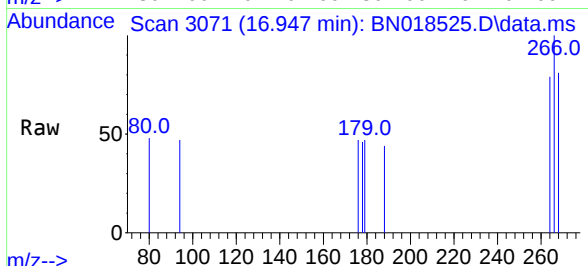

Tgt Ion:266 Resp: 129

Ion	Ratio	Lower	Upper
266	100		
264	63.6	49.9	74.9
268	64.3	51.7	77.5

