

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018526.D
 Acq On : 01 Feb 2022 22:47
 Operator : CG/JU
 Sample : PB142388BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK388

Quant Time: Feb 02 04:47:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	380	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1364	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	792	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.293	188	1526	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.464	240	1205	0.400	ng/ul	# 0.00
23) Perylene-d12	23.858	264	1274	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2811	6.422	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.322	152	715	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.318	212	1490	0.443	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.947	266	118	0.870	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018526.D
Acq On : 01 Feb 2022 22:47
Operator : CG/JU
Sample : PB142388BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388


Quant Time: Feb 02 04:47:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration

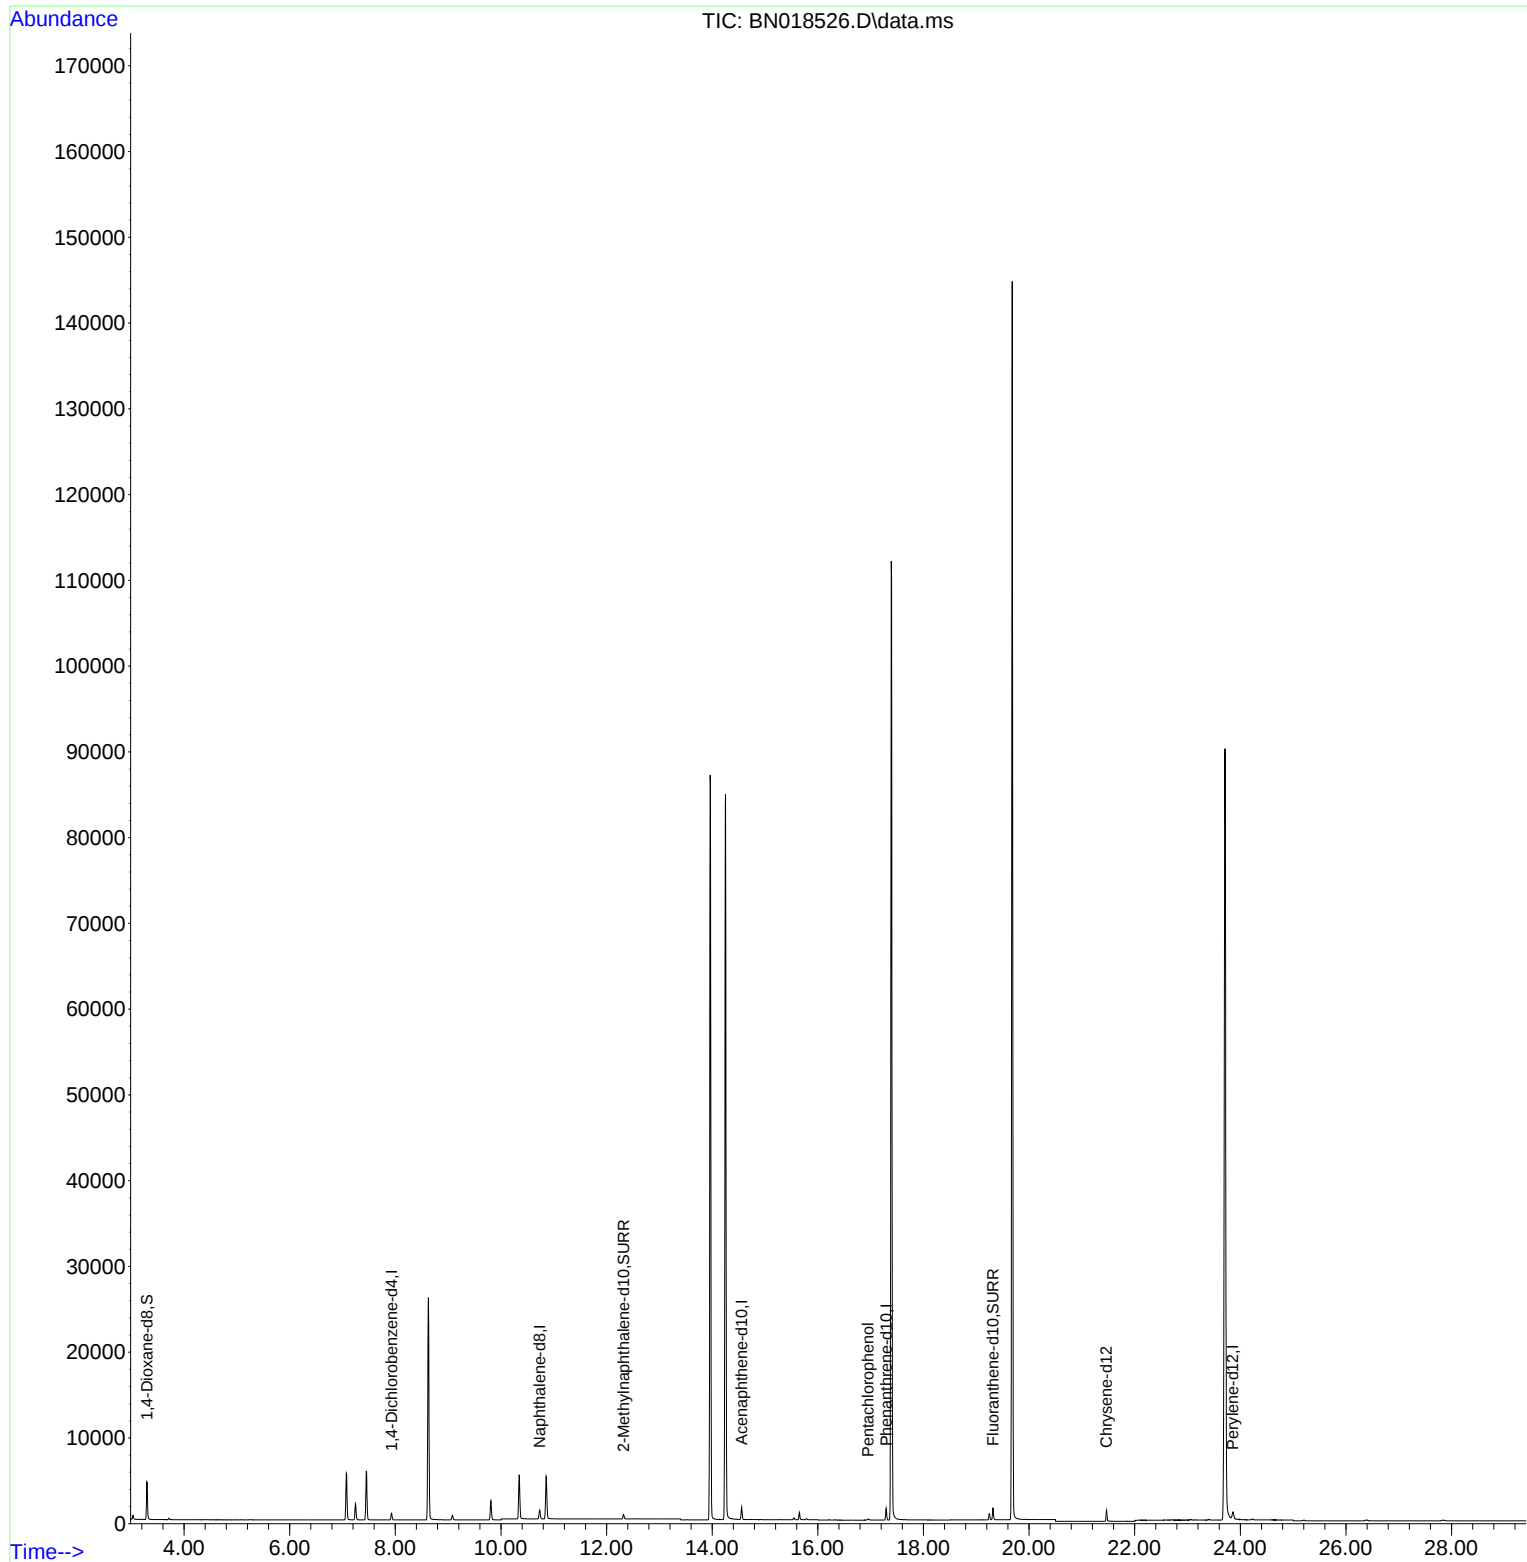

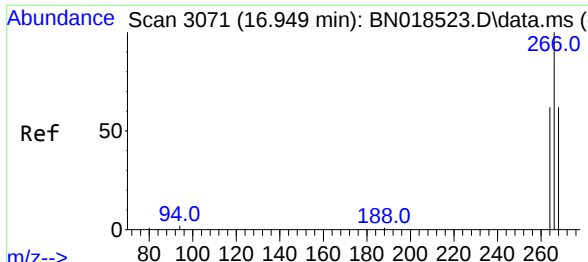

#14
Pentachlorophenol
Concen: 0.870 ng/ul
RT: 16.947 min Scan# 30
Delta R.T. -0.001 min
Lab File: BN018526.D
Acq: 01 Feb 2022 22:47

Instrument :
BNA_N
ClientSampleId :
SBLK388

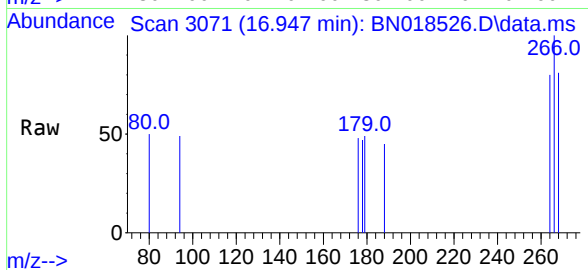

Tgt Ion:266 Resp: 118

Ion	Ratio	Lower	Upper
266	100		
264	61.9	49.9	74.9
268	66.1	51.7	77.5

