

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018534.D
 Acq On : 02 Feb 2022 03:31
 Operator : CG/JU
 Sample : N1307-18
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q61

Quant Time: Feb 02 05:56:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	403	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136	1468	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.555	164	880	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188	1744	0.400	ng/ul #	0.00
17) Chrysene-d12	21.463	240	1478	0.400	ng/ul #	0.00
23) Perylene-d12	23.857	264	1478	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2003	4.315	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.319	152	839	0.424	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	2170	0.526	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.638	153	178	0.059	ng/ul#	53
14) Pentachlorophenol	16.945	266	569	3.671	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018534.D
Acq On : 02 Feb 2022 03:31
Operator : CG/JU
Sample : N1307-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q61

Quant Time: Feb 02 05:56:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration




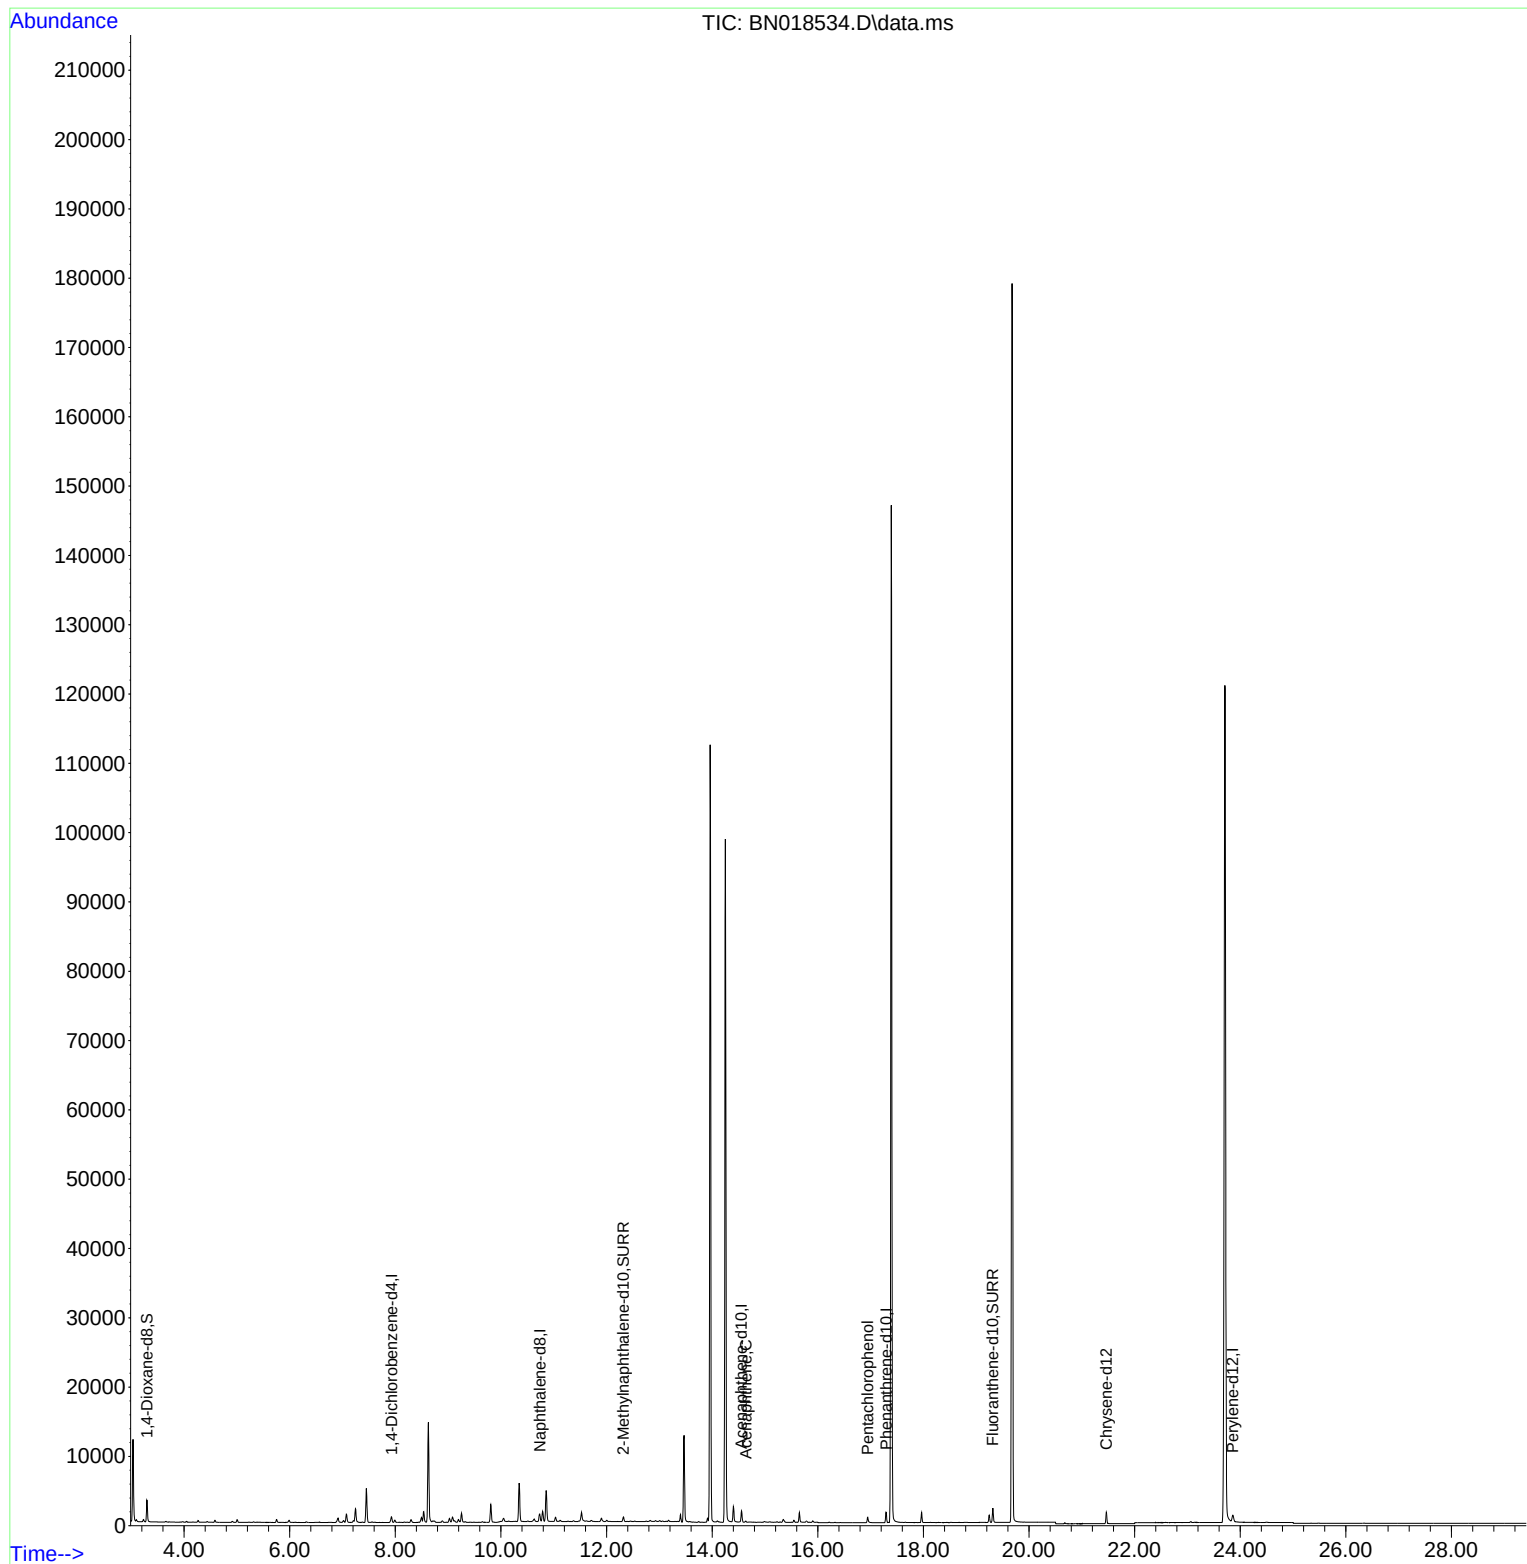


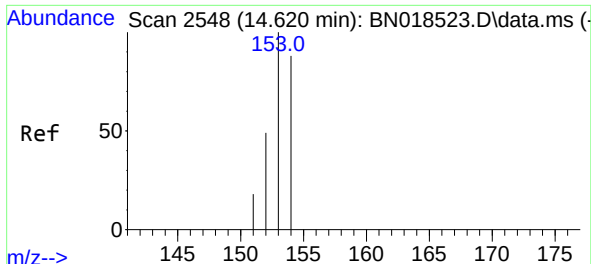

#11
Acenaphthene
Concen: 0.059 ng/ul
RT: 14.638 min Scan# 2552
Delta R.T. 0.018 min
Lab File: BN018534.D
Acq: 02 Feb 2022 03:31

Instrument :
BNA_N
ClientSampleId :
C0Q61

Tgt Ion:153 Resp: 178
Ion Ratio Lower Upper
153 100
152 30.1 39.7 59.5#
154 34.7 70.9 106.3#

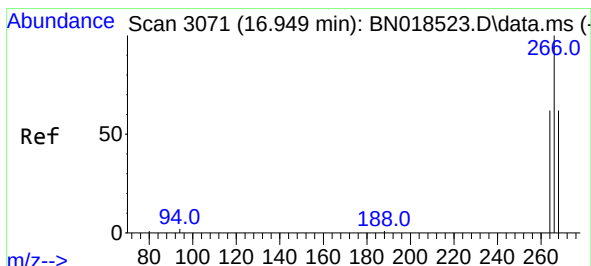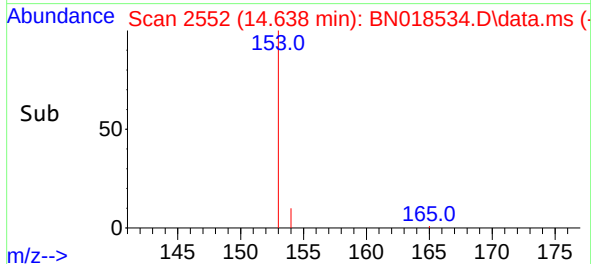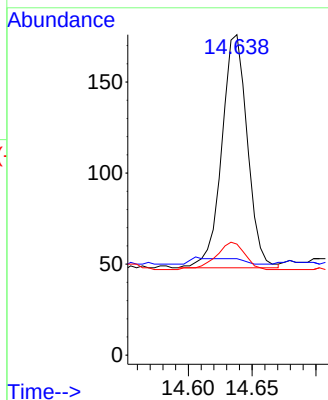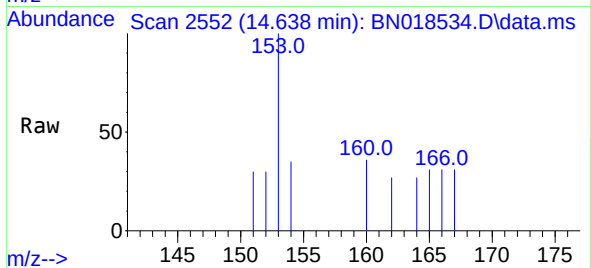

#14
Pentachlorophenol
Concen: 3.671 ng/ul
RT: 16.945 min Scan# 3070
Delta R.T. -0.004 min
Lab File: BN018534.D
Acq: 02 Feb 2022 03:31

Tgt Ion:266 Resp: 569
Ion Ratio Lower Upper
266 100
264 61.5 49.9 74.9
268 63.4 51.7 77.5

