

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023905.D
 Acq On : 02 Feb 2023 15:12
 Operator : CG/JU
 Sample : 01362-04DL 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4442DL

Quant Time: Feb 03 01:18:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	141299	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	616957	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	422982	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.257	188	1032526	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	935681	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	982272	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	460	0.131	ng/uL	0.00
4) Pyridine-d5	3.664	84	113	0.012	ng/ul	0.00
7) Phenol-d5	7.022	99	7261	0.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	5457	0.700	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	5859	0.607	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	5854	0.598	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	2824	0.564	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	2671	0.469	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	6725	0.632	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	8436	0.581	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	23958	0.709	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	23060	0.631	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	1418	0.232	ng/ul	0.00
60) Fluorene-d10	15.498	176	22066	0.779	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	1023	0.140	ng/ul	0.00
73) Anthracene-d10	17.351	188	33821	0.704	ng/ul	0.00
81) Pyrene-d10	19.645	212	42620	0.750	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	38386	0.753	ng/ul	-0.01


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.363	149	2584161	62.263 ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023905.D
Acq On : 02 Feb 2023 15:12
Operator : CG/JU
Sample : 01362-04DL 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4442DL

Quant Time: Feb 03 01:18:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

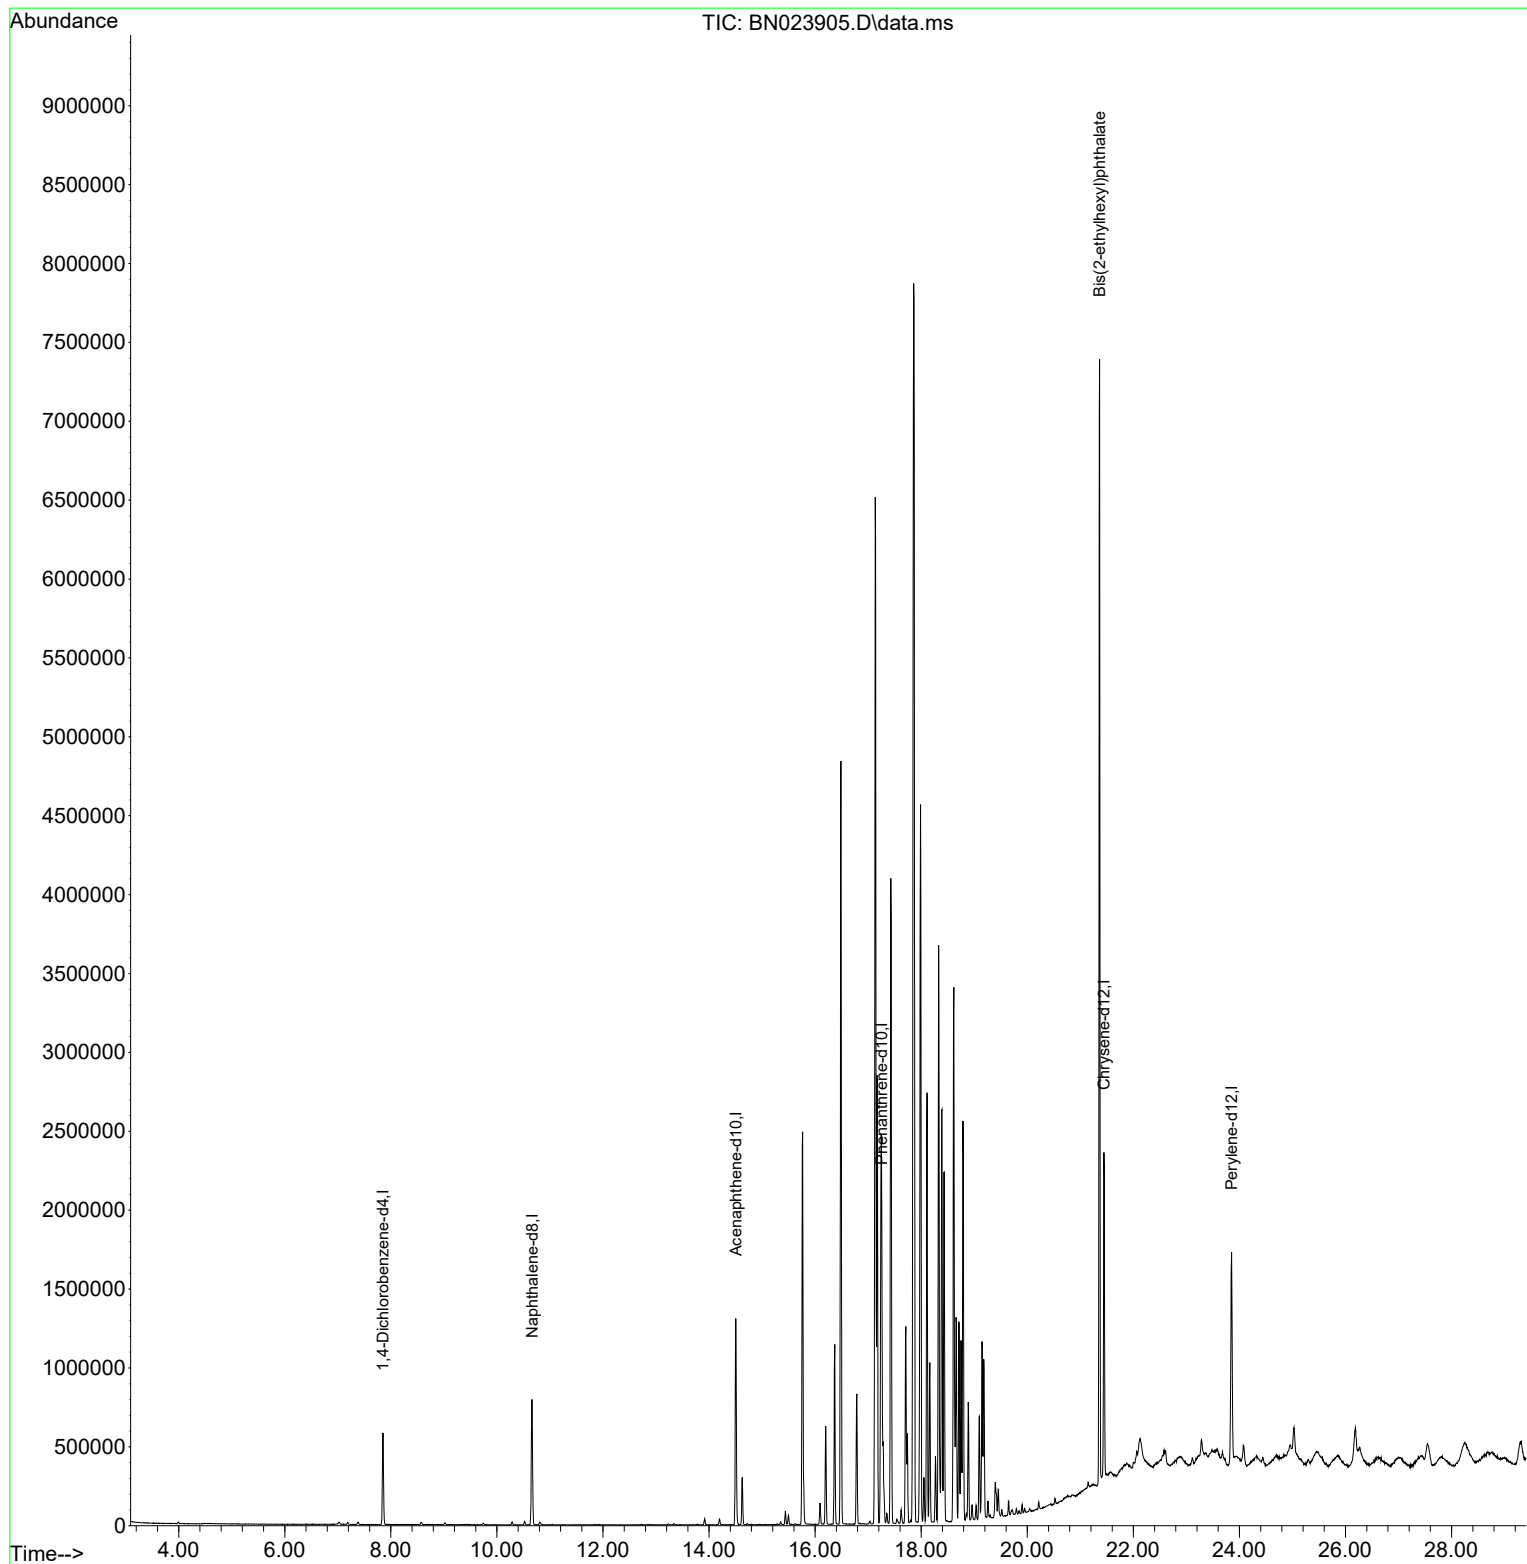

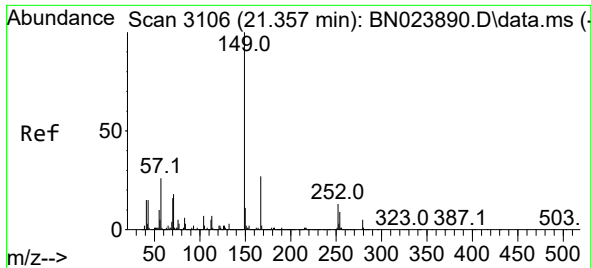

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 62.263 ng/ul
 RT: 21.363 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BN023905.D
 Acq: 02 Feb 2023 15:12

Instrument :
 BNA_N
 ClientSampleId :
 A4442DL

Tgt Ion:149 Resp: 2584161
 Ion Ratio Lower Upper
 149 100
 167 28.9 21.2 31.8
 279 4.7 3.8 5.6

