

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023906.D
 Acq On : 02 Feb 2023 15:49
 Operator : CG/JU
 Sample : 01362-05DL 30X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4443DL

Quant Time: Feb 03 01:18:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	138592	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	608997	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	416531	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.257	188	1024316	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	875699	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	871229	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	700	0.204	ng/uL	0.00
4) Pyridine-d5	3.664	84	179	0.019	ng/ul	0.00
7) Phenol-d5	7.022	99	3943	0.326	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	3478	0.455	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	3522	0.372	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	3333	0.347	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	1792	0.363	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	1851	0.329	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	3775	0.360	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	4170	0.291	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	14748	0.443	ng/ul	0.00
49) Acenaphthylene-d8	14.193	160	14027	0.390	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	527	0.087	ng/ul	0.00
60) Fluorene-d10	15.498	176	14381	0.516	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	564	0.078	ng/ul	0.00
73) Anthracene-d10	17.351	188	19236	0.403	ng/ul	0.00
81) Pyrene-d10	19.645	212	23930	0.450	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	21909	0.485	ng/ul	-0.01


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.369	149	5969093	153.672 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023906.D
Acq On : 02 Feb 2023 15:49
Operator : CG/JU
Sample : 01362-05DL 30X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4443DL

Quant Time: Feb 03 01:18:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

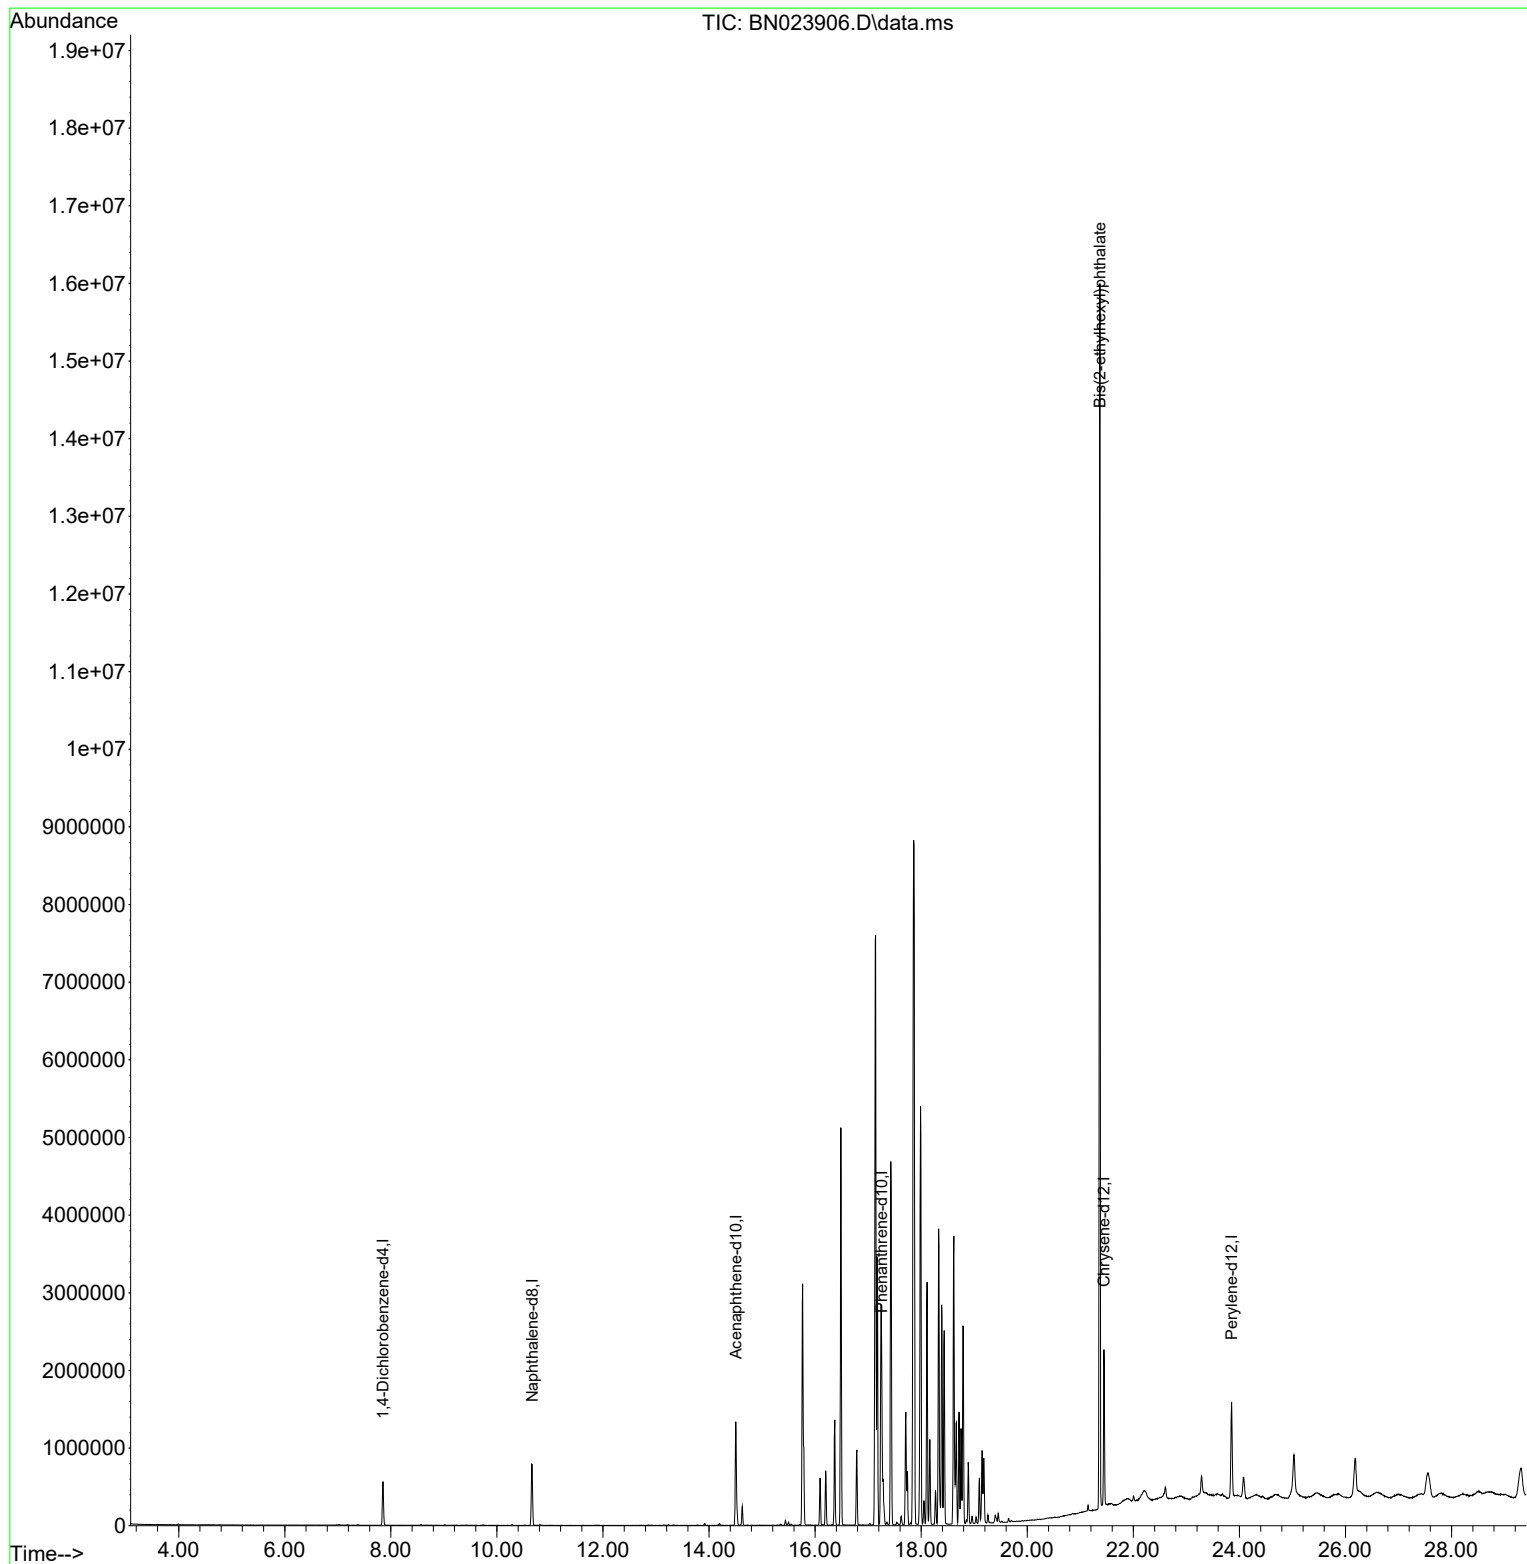

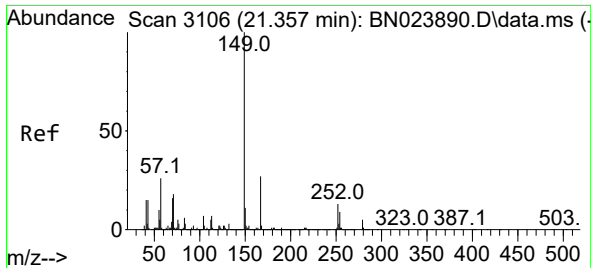

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 153.672 ng/ul
 RT: 21.369 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BN023906.D
 Acq: 02 Feb 2023 15:49

Instrument :
 BNA_N
 ClientSampleId :
 A4443DL

Tgt Ion:149 Resp: 5969093
 Ion Ratio Lower Upper
 149 100
 167 27.4 21.2 31.8
 279 5.7 3.8 5.6#

