

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023910.D
 Acq On : 02 Feb 2023 18:21
 Operator : CG/JU
 Sample : PB150495BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Quant Time: Feb 03 01:19:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	144483	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	612337	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	423443	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	971308	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	848196	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	835406	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	20224	5.649	ng/uL	0.00
4) Pyridine-d5	3.663	84	271769	27.171	ng/ul	0.00
7) Phenol-d5	7.022	99	339260	26.889	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	220707	27.679	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	274901	27.865	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	276787	27.654	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	136178	27.410	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	157769	27.910	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	282848	26.797	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	401918	27.912	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1027884	30.405	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1046051	28.604	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	157487	25.695	ng/ul	0.00
60) Fluorene-d10	15.498	176	830260	29.295	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	148245	21.569	ng/ul	0.00
73) Anthracene-d10	17.351	188	1405620	31.084	ng/ul	0.00
81) Pyrene-d10	19.651	212	1576064	30.605	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	1366020	31.505	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.362	149	72540	1.928 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023910.D
Acq On : 02 Feb 2023 18:21
Operator : CG/JU
Sample : PB150495BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Time: Feb 03 01:19:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

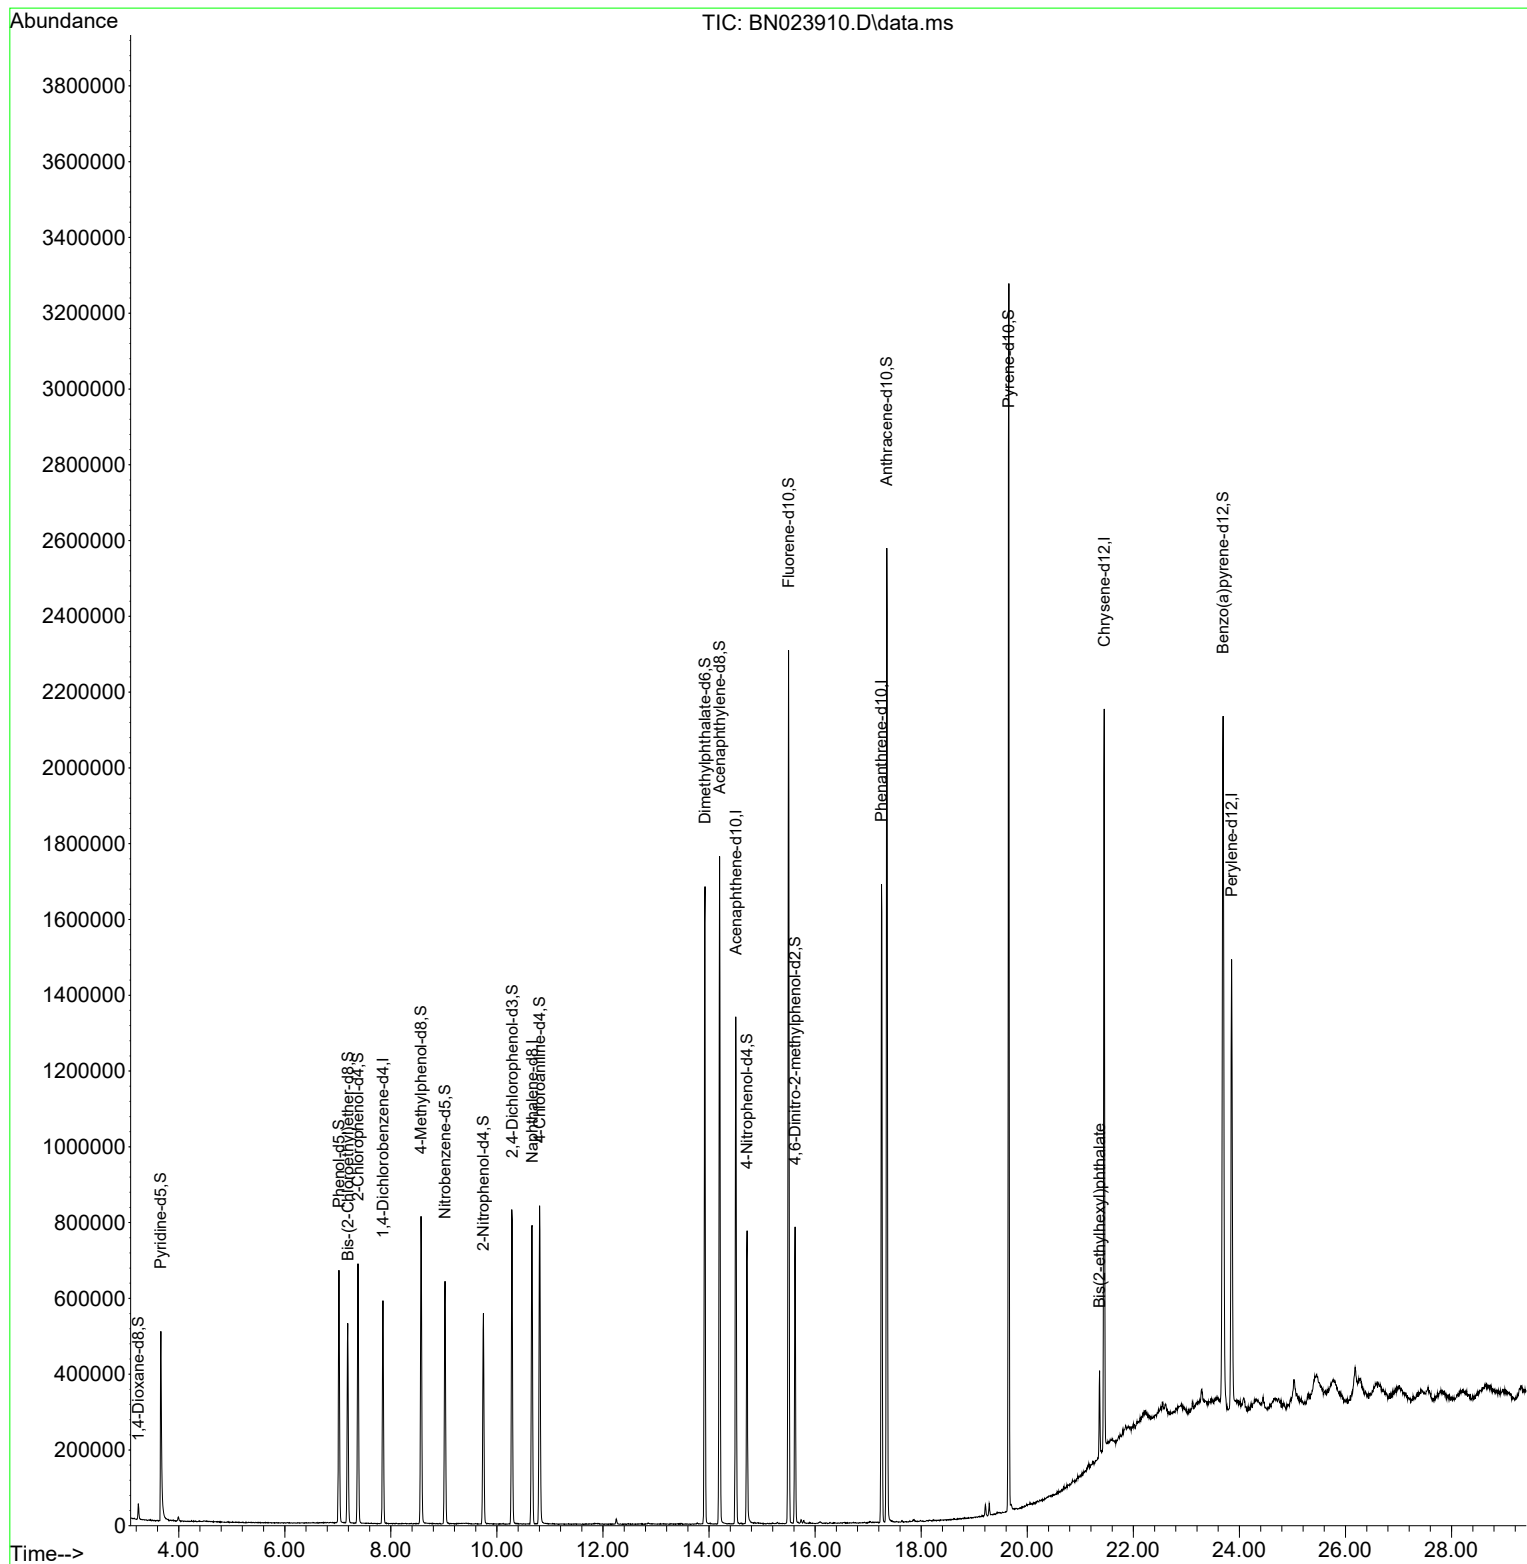

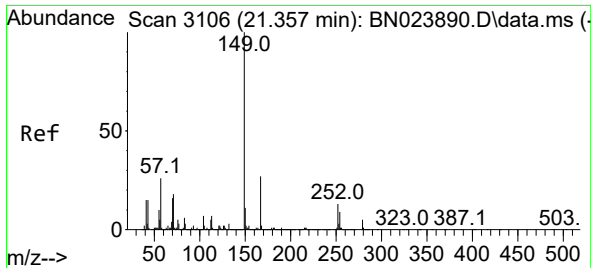

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.928 ng/ul
 RT: 21.362 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BN023910.D
 Acq: 02 Feb 2023 18:21

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Tgt Ion:149 Resp: 72540
 Ion Ratio Lower Upper
 149 100
 167 27.1 21.2 31.8
 279 4.6 3.8 5.6

