

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023911.D
 Acq On : 02 Feb 2023 18:58
 Operator : CG/JU
 Sample : PB150496BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK496

Quant Time: Feb 03 01:19:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	132961	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	555150	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	380613	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	865298	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	764726	20.000	ng/ul	0.00
88) Perylene-d12	23.839	264	731772	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	22146	6.722	ng/uL	0.00
4) Pyridine-d5	3.664	84	300198	32.614	ng/ul	0.00
7) Phenol-d5	7.022	99	372510	32.083	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	243038	33.121	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	304427	33.532	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	309014	33.550	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	150020	33.307	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	176111	34.363	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	314358	32.850	ng/ul	0.00
31) 4-Chloroaniline-d4	10.805	131	442560	33.900	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1105461	36.379	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1145611	34.851	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	175651	31.883	ng/ul	0.00
60) Fluorene-d10	15.498	176	921450	36.171	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	174993	28.579	ng/ul	0.00
73) Anthracene-d10	17.351	188	1507266	37.416	ng/ul	0.00
81) Pyrene-d10	19.651	212	1737132	37.415	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1475173	38.840	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.357	149	66823	1.970	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023911.D
Acq On : 02 Feb 2023 18:58
Operator : CG/JU
Sample : PB150496BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK496

Quant Time: Feb 03 01:19:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

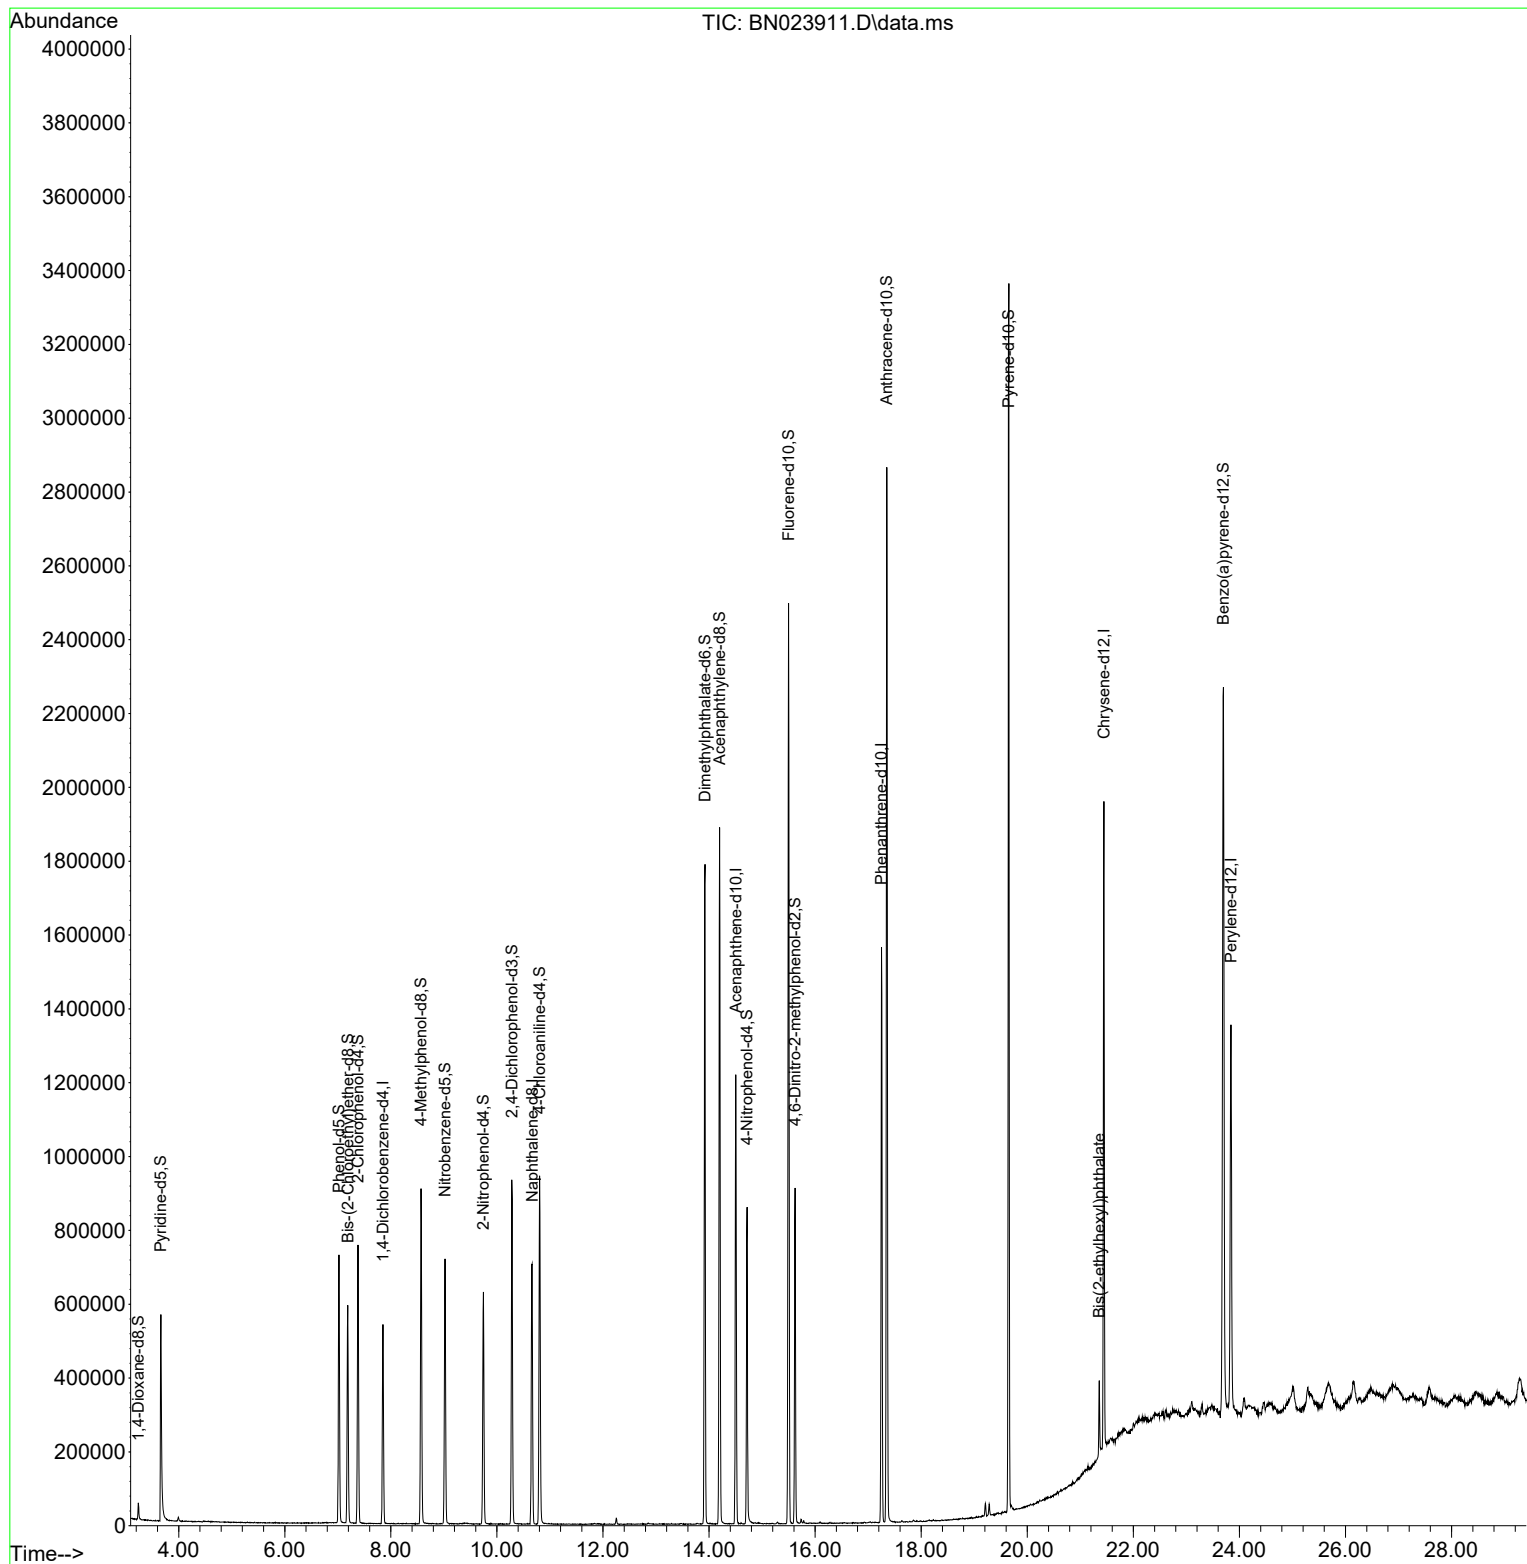

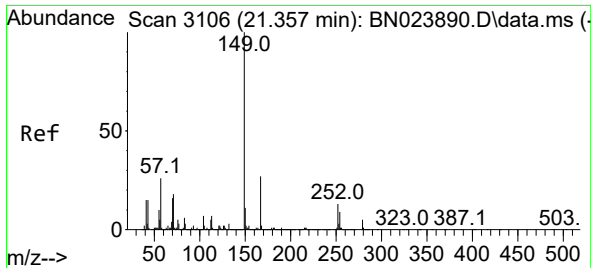

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.970 ng/ul
 RT: 21.357 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN023911.D
 Acq: 02 Feb 2023 18:58

Instrument :
 BNA_N
 ClientSampleId :
 SBLK496

Tgt Ion:149 Resp: 66823
 Ion Ratio Lower Upper
 149 100
 167 25.6 21.2 31.8
 279 5.2 3.8 5.6

