

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023914.D
 Acq On : 02 Feb 2023 20:49
 Operator : CG/JU
 Sample : 01294-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P1

Quant Time: Feb 03 01:21:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	150493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	617830	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	418199	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	946132	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	815231	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264	765504	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	18370	4.927	ng/uL	0.00
4) Pyridine-d5	3.664	84	105821	10.157	ng/ul	0.00
7) Phenol-d5	7.022	99	76094	5.790	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	257442	30.997	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	243514	23.698	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	153983	14.770	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	162727	32.463	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	176311	30.912	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	311779	29.276	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	262798	18.088	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1280580	38.355	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1272747	35.239	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	31775	5.249	ng/ul	0.00
60) Fluorene-d10	15.498	176	1038795	37.113	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	220480	32.932	ng/ul	0.00
73) Anthracene-d10	17.351	188	1711596	38.858	ng/ul	0.00
81) Pyrene-d10	19.651	212	2050002	41.418	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	1552413	39.073	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.063	77	569042	45.219	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.357	149	67871	1.877	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023914.D
Acq On : 02 Feb 2023 20:49
Operator : CG/JU
Sample : 01294-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P1

Quant Time: Feb 03 01:21:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration




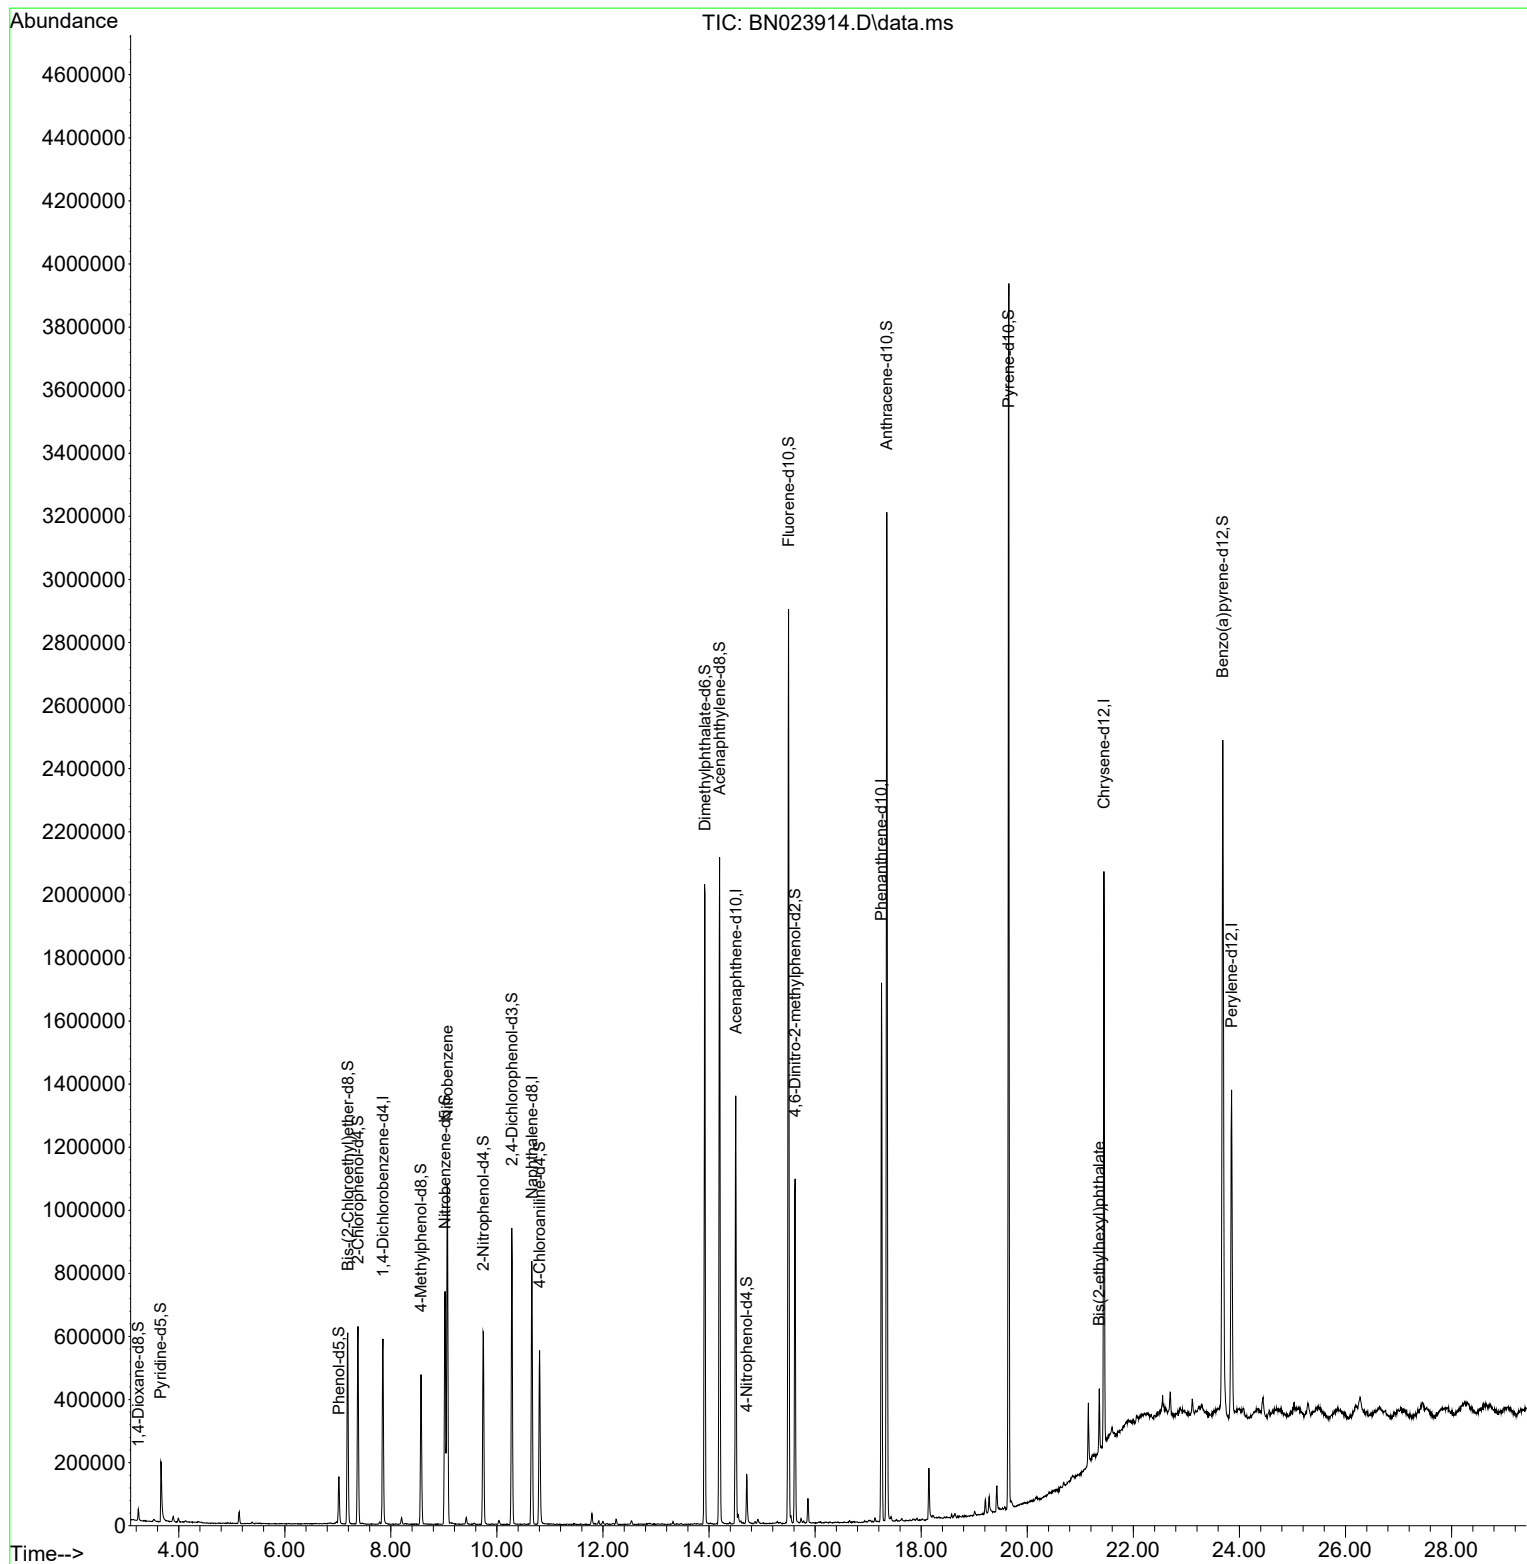


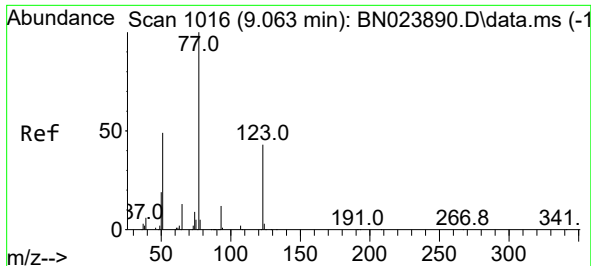

#22
Nitrobenzene
Concen: 45.219 ng/ul
RT: 9.063 min Scan# 1016
Delta R.T. -0.000 min
Lab File: BN023914.D
Acq: 02 Feb 2023 20:49

Instrument :
BNA_N
ClientSampleId :
A44P1

Tgt Ion: 77 Resp: 569042
Ion Ratio Lower Upper
77 100
123 43.0 34.2 51.2
65 13.7 10.9 16.3

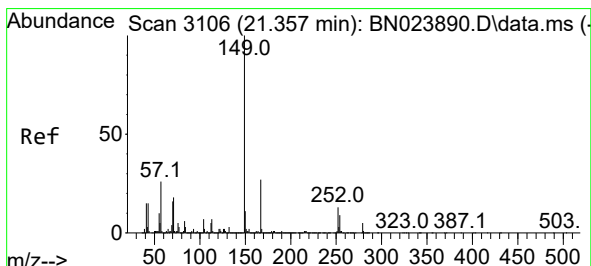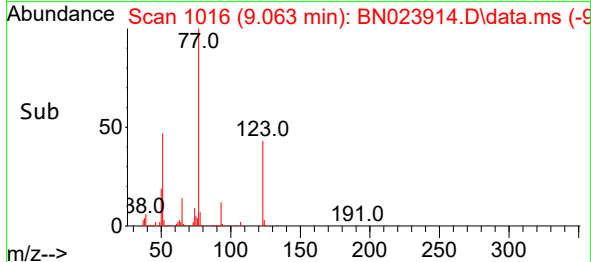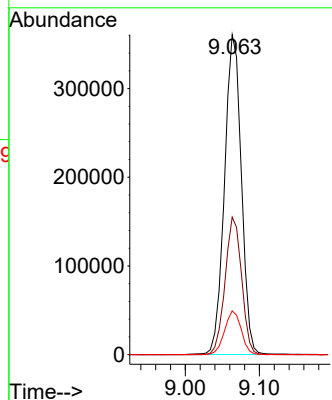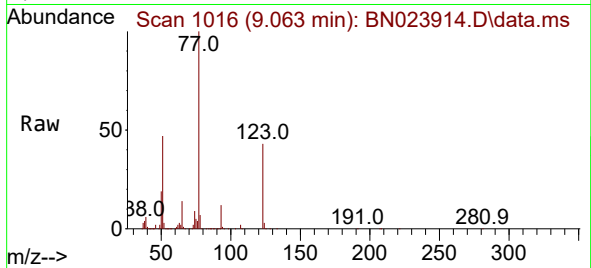

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.877 ng/ul
RT: 21.357 min Scan# 3106
Delta R.T. -0.000 min
Lab File: BN023914.D
Acq: 02 Feb 2023 20:49

Tgt Ion: 149 Resp: 67871
Ion Ratio Lower Upper
149 100
167 27.8 21.2 31.8
279 4.4 3.8 5.6

