

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023915.D
 Acq On : 02 Feb 2023 21:26
 Operator : CG/JU
 Sample : 01294-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P3

Quant Time: Feb 03 01:21:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	158049	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	670725	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	458747	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	1061160	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	937749	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	886588	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	16788	4.287	ng/uL	0.00
4) Pyridine-d5	3.664	84	82361	7.527	ng/ul	0.00
7) Phenol-d5	7.022	99	78610	5.696	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	244483	28.029	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	235961	21.865	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	154454	14.107	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	153709	28.245	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	167383	27.033	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	290587	25.134	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	384793	24.396	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1128515	30.813	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1202266	30.345	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	30263	4.558	ng/ul	0.00
60) Fluorene-d10	15.498	176	982968	32.014	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	195048	25.975	ng/ul	0.00
73) Anthracene-d10	17.351	188	1660547	33.612	ng/ul	0.00
81) Pyrene-d10	19.651	212	1925156	33.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1591098	34.577	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.357	149	51472	1.237	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023915.D
Acq On : 02 Feb 2023 21:26
Operator : CG/JU
Sample : 01294-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P3

Quant Time: Feb 03 01:21:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

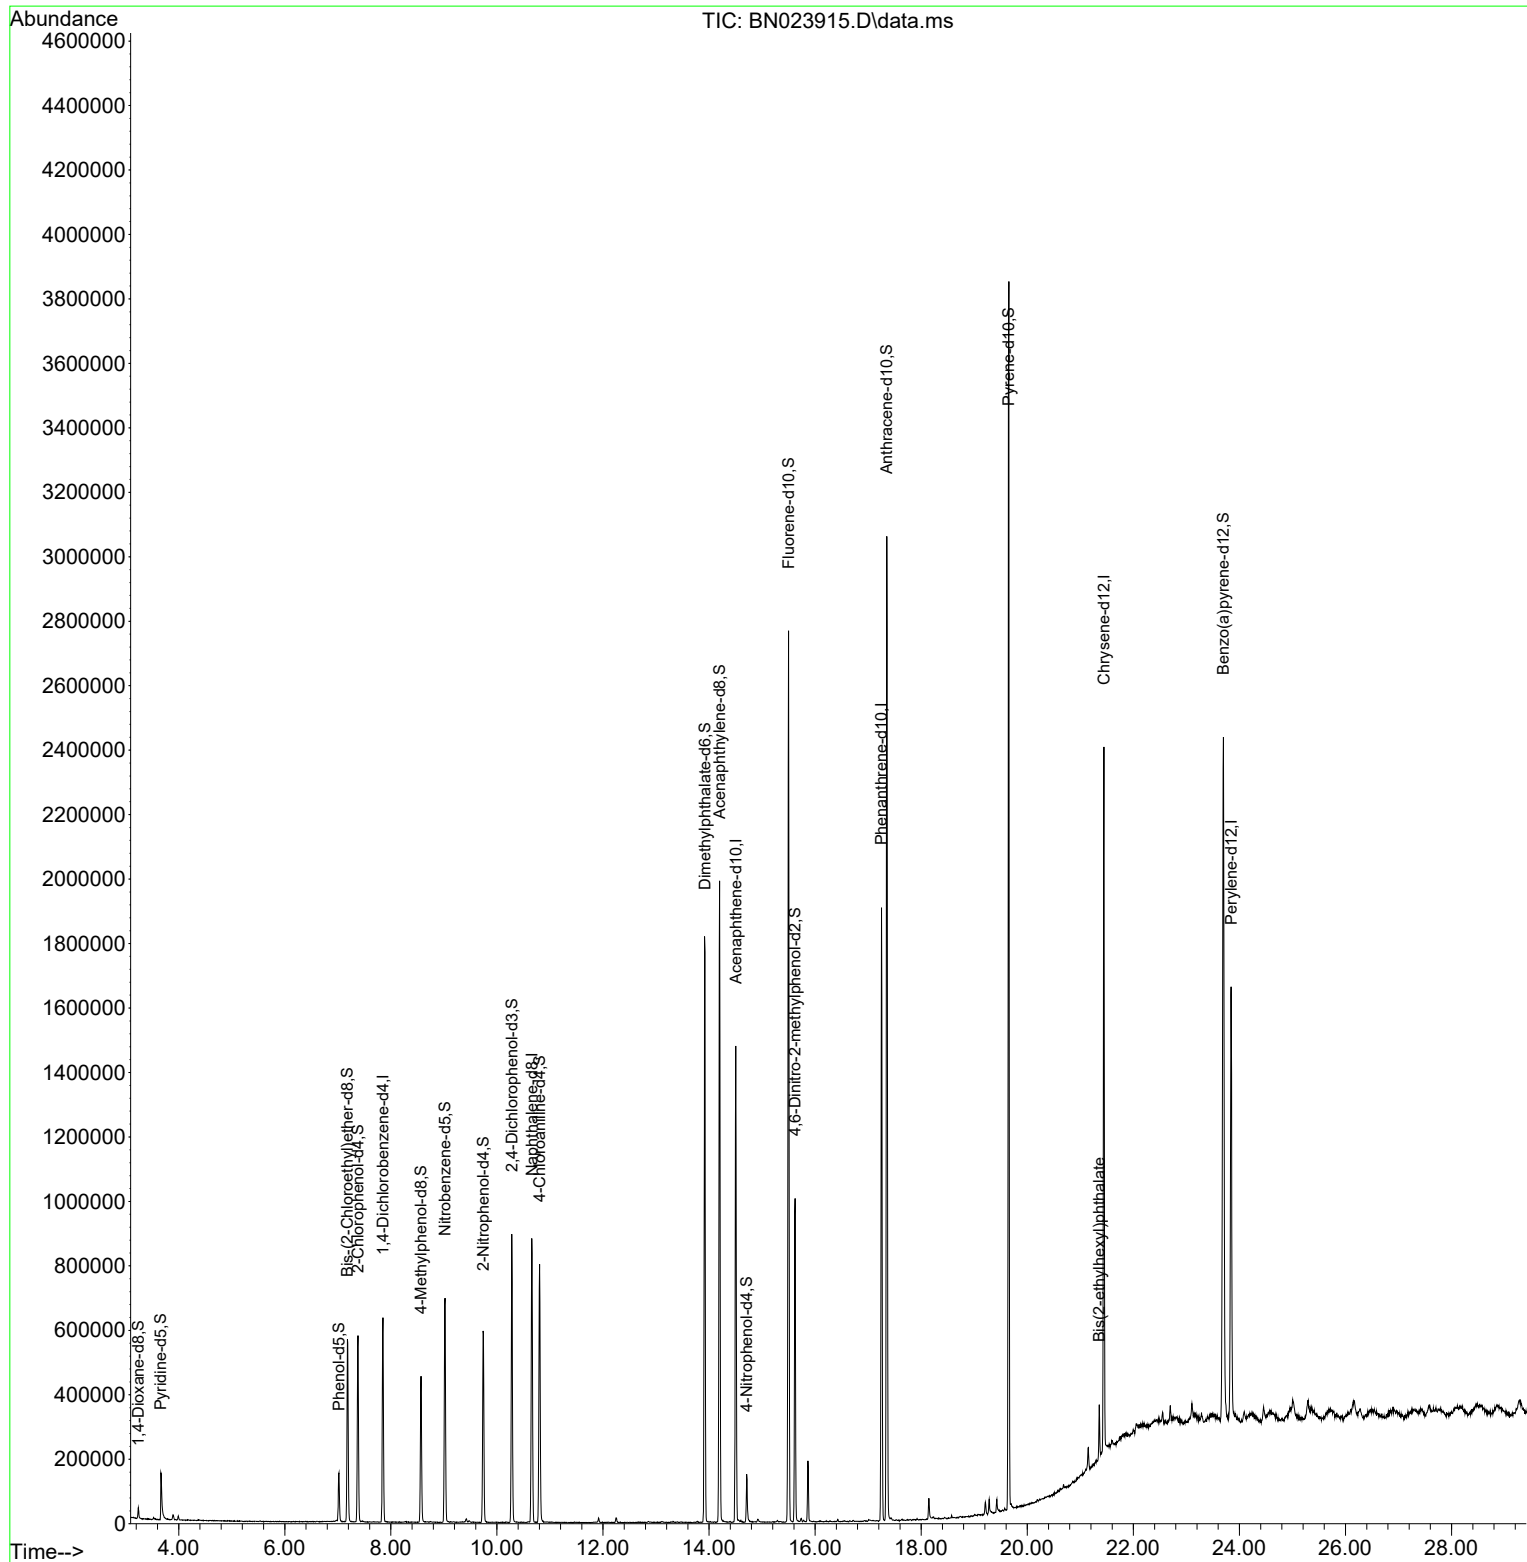

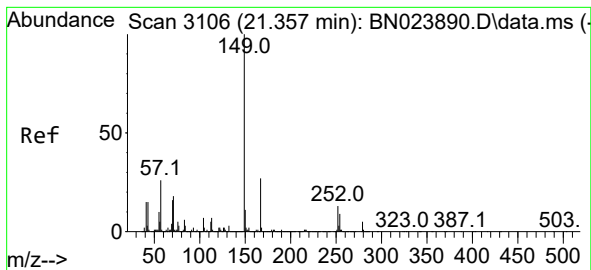

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.237 ng/ul
 RT: 21.357 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN023915.D
 Acq: 02 Feb 2023 21:26

Instrument :
 BNA_N
 ClientSampleId :
 A44P3

Tgt Ion:149 Resp: 51472
 Ion Ratio Lower Upper
 149 100
 167 25.8 21.2 31.8
 279 5.1 3.8 5.6

