

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023916.D
 Acq On : 02 Feb 2023 22:03
 Operator : CG/JU
 Sample : 01294-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P4

Quant Time: Feb 03 01:21:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	147568	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	623769	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	420864	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	967851	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	893446	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	836875	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	17084	4.672	ng/uL	0.00
4) Pyridine-d5	3.664	84	87587	8.574	ng/ul	0.00
7) Phenol-d5	7.022	99	81767	6.345	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	256692	31.519	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	249061	24.718	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	161555	15.804	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	160546	31.723	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	177080	30.752	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	302526	28.136	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	404733	27.592	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	1229098	36.580	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1243415	34.209	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	35025	5.750	ng/ul	0.00
60) Fluorene-d10	15.498	176	1043054	37.029	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	223579	32.645	ng/ul	0.00
73) Anthracene-d10	17.351	188	1814196	40.263	ng/ul	0.00
81) Pyrene-d10	19.651	212	2132301	39.310	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	1819139	41.881	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.351	149	48456	1.223	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023916.D
Acq On : 02 Feb 2023 22:03
Operator : CG/JU
Sample : 01294-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P4

Quant Time: Feb 03 01:21:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

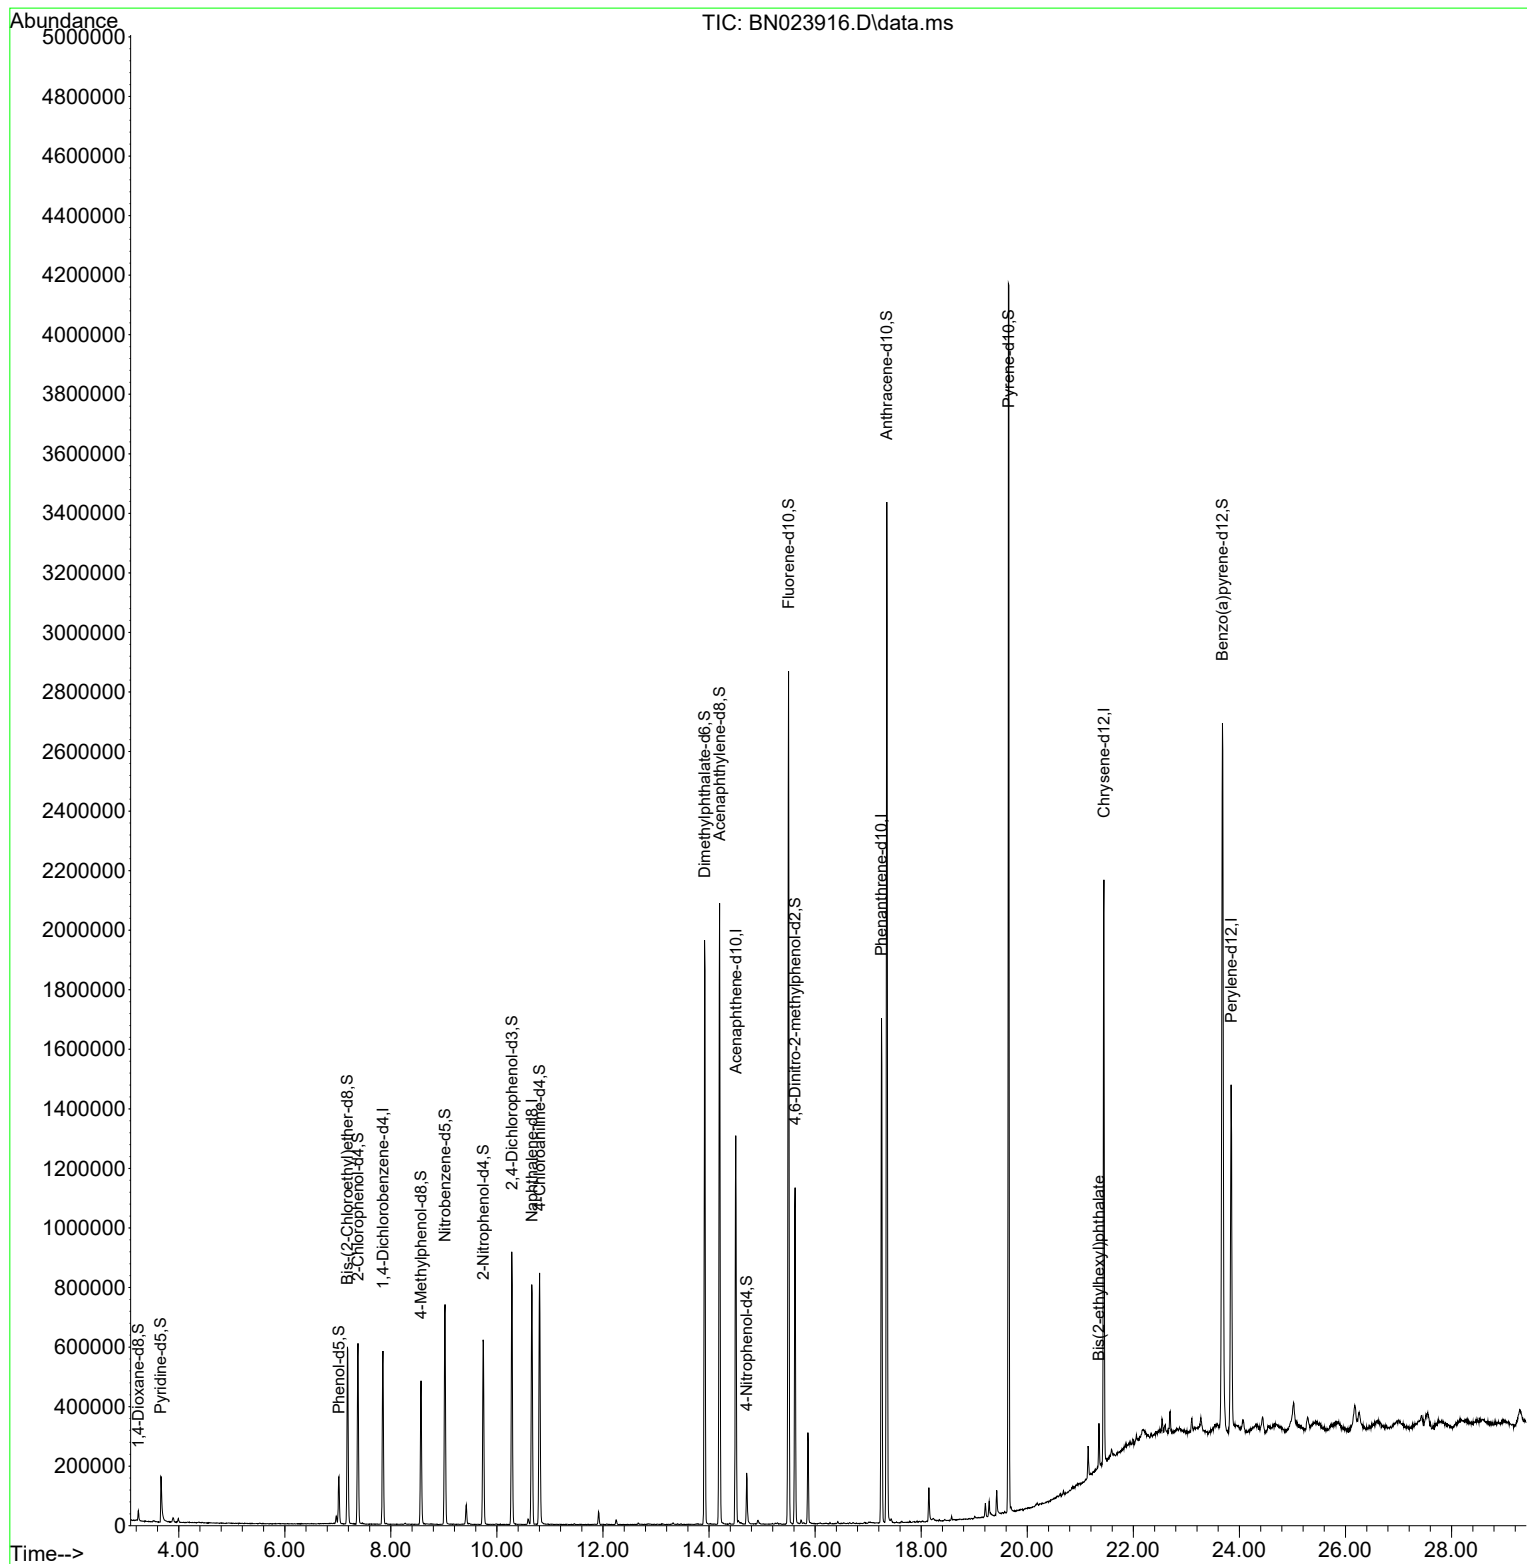

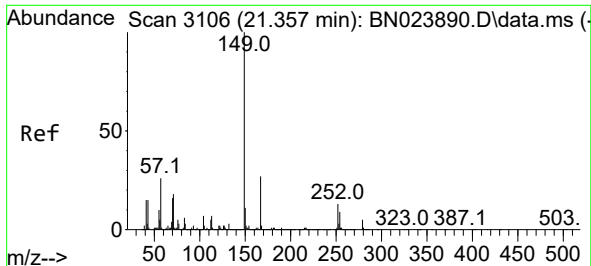

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.223 ng/ul
 RT: 21.351 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN023916.D
 Acq: 02 Feb 2023 22:03

Instrument :
 BNA_N
 ClientSampleId :
 A44P4

Tgt Ion:149 Resp: 48456
 Ion Ratio Lower Upper
 149 100
 167 27.1 21.2 31.8
 279 5.3 3.8 5.6

