

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023919.D
 Acq On : 02 Feb 2023 23:53
 Operator : CG/JU
 Sample : 01294-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44N6

Quant Time: Feb 03 01:21:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	151442	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	642930	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	432261	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	965353	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	837767	20.000	ng/ul	-0.01
88) Perylene-d12	23.833	264	769475	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	18496	4.929	ng/uL	0.00
4) Pyridine-d5	3.664	84	107274	10.232	ng/ul	0.00
7) Phenol-d5	7.016	99	84306	6.375	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	285246	34.129	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	262002	25.338	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	167138	15.932	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	172704	33.108	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	189170	31.872	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	327557	29.556	ng/ul	0.00
31) 4-Chloroaniline-d4	10.805	131	417722	27.629	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166	1328278	38.489	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	1344219	36.007	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	33174	5.302	ng/ul	0.00
60) Fluorene-d10	15.498	176	1128564	39.008	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	222053	32.506	ng/ul	0.00
73) Anthracene-d10	17.351	188	1885244	41.948	ng/ul	0.00
81) Pyrene-d10	19.651	212	2178626	42.833	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	1780115	44.573	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.357	149	42981	1.157	ng/ul#	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023919.D
Acq On : 02 Feb 2023 23:53
Operator : CG/JU
Sample : 01294-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44N6

Quant Time: Feb 03 01:21:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

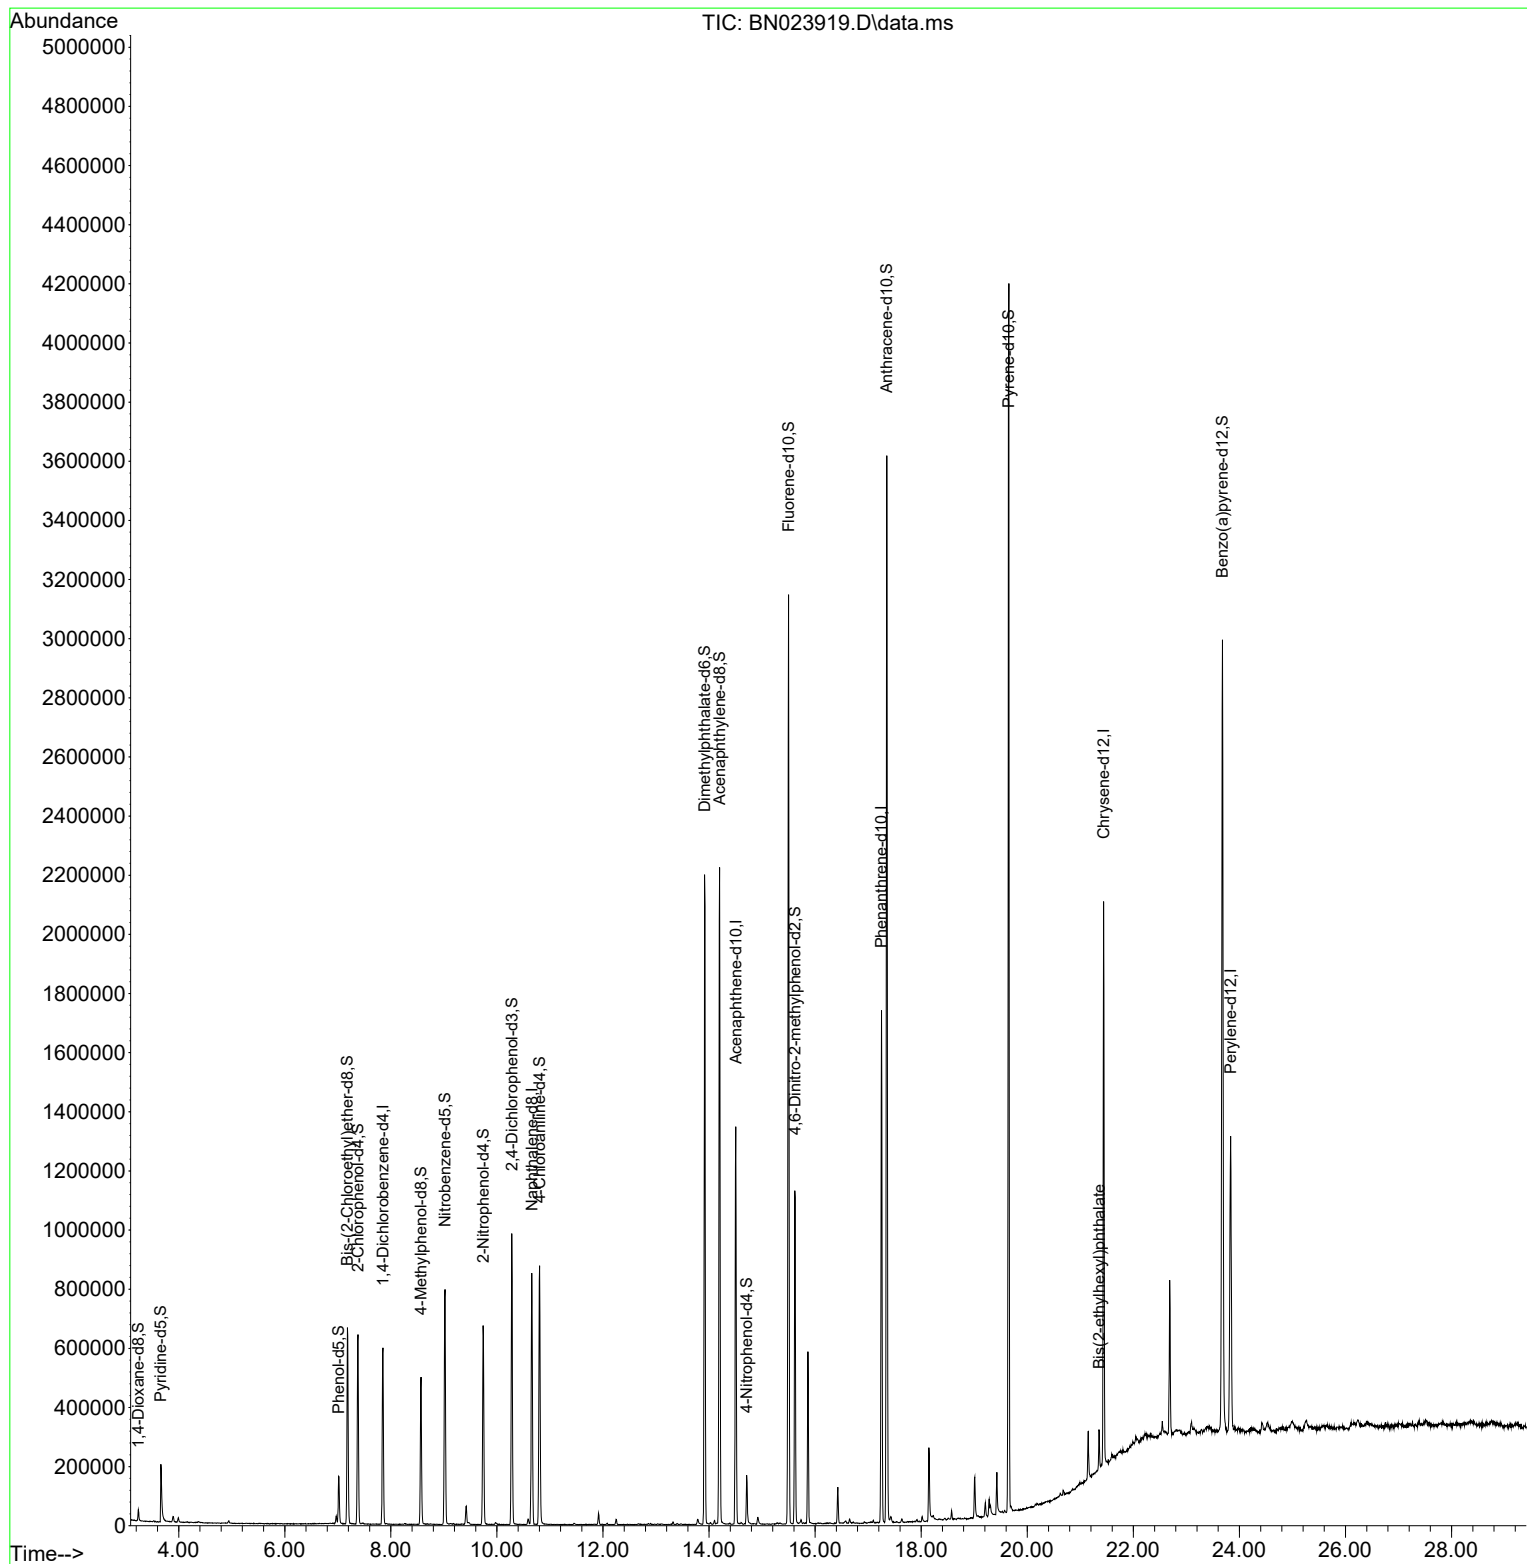

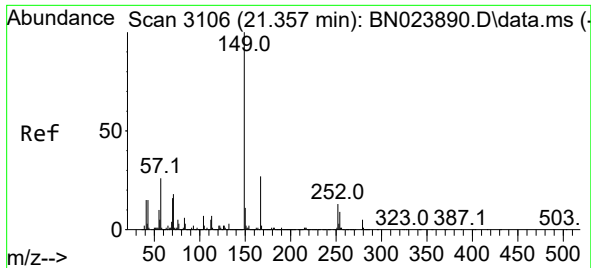

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.157 ng/ul
 RT: 21.357 min Scan# 3106
 Delta R.T. -0.000 min
 Lab File: BN023919.D
 Acq: 02 Feb 2023 23:53

Instrument :
 BNA_N
 ClientSampleId :
 A44N6

Tgt Ion:149 Resp: 42981
 Ion Ratio Lower Upper
 149 100
 167 29.2 21.2 31.8
 279 6.7 3.8 5.6#

