

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023933.D
 Acq On : 03 Feb 2023 09:02
 Operator : CG/JU
 Sample : 01295-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC9

Quant Time: Feb 03 21:50:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	151179	20.000	ng/u1	0.00
20) Naphthalene-d8	10.658	136	642390	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.499	164	437958	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	985469	20.000	ng/u1	0.00
79) Chrysene-d12	21.445	240	891003	20.000	ng/u1	0.00
88) Perylene-d12	23.851	264	849789	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	16645	4.444	ng/uL	0.00
4) Pyridine-d5	3.664	84	99527	9.510	ng/u1	0.00
7) Phenol-d5	7.017	99	59998	4.545	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	230061	27.574	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	180112	17.448	ng/u1	0.00
15) 4-Methylphenol-d8	8.564	113	116218	11.097	ng/u1	-0.01
21) Nitrobenzene-d5	9.016	128	146272	28.064	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	127288	21.464	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	224735	20.295	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.799	131	382582	25.326	ng/u1	-0.01
46) Dimethylphthalate-d6	13.916	166	1082447	30.958	ng/u1	0.00
49) Acenaphthylene-d8	14.193	160	1132283	29.936	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	22422	3.537	ng/u1	0.00
60) Fluorene-d10	15.493	176	945744	32.264	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	145356	20.844	ng/u1	0.00
73) Anthracene-d10	17.345	188	1629979	35.528	ng/u1	0.00
81) Pyrene-d10	19.645	212	1965367	36.332	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1612875	36.568	ng/u1	-0.01


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.276	88	8995	2.331	ng/uL#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023933.D
Acq On : 03 Feb 2023 09:02
Operator : CG/JU
Sample : 01295-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC9

Quant Time: Feb 03 21:50:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

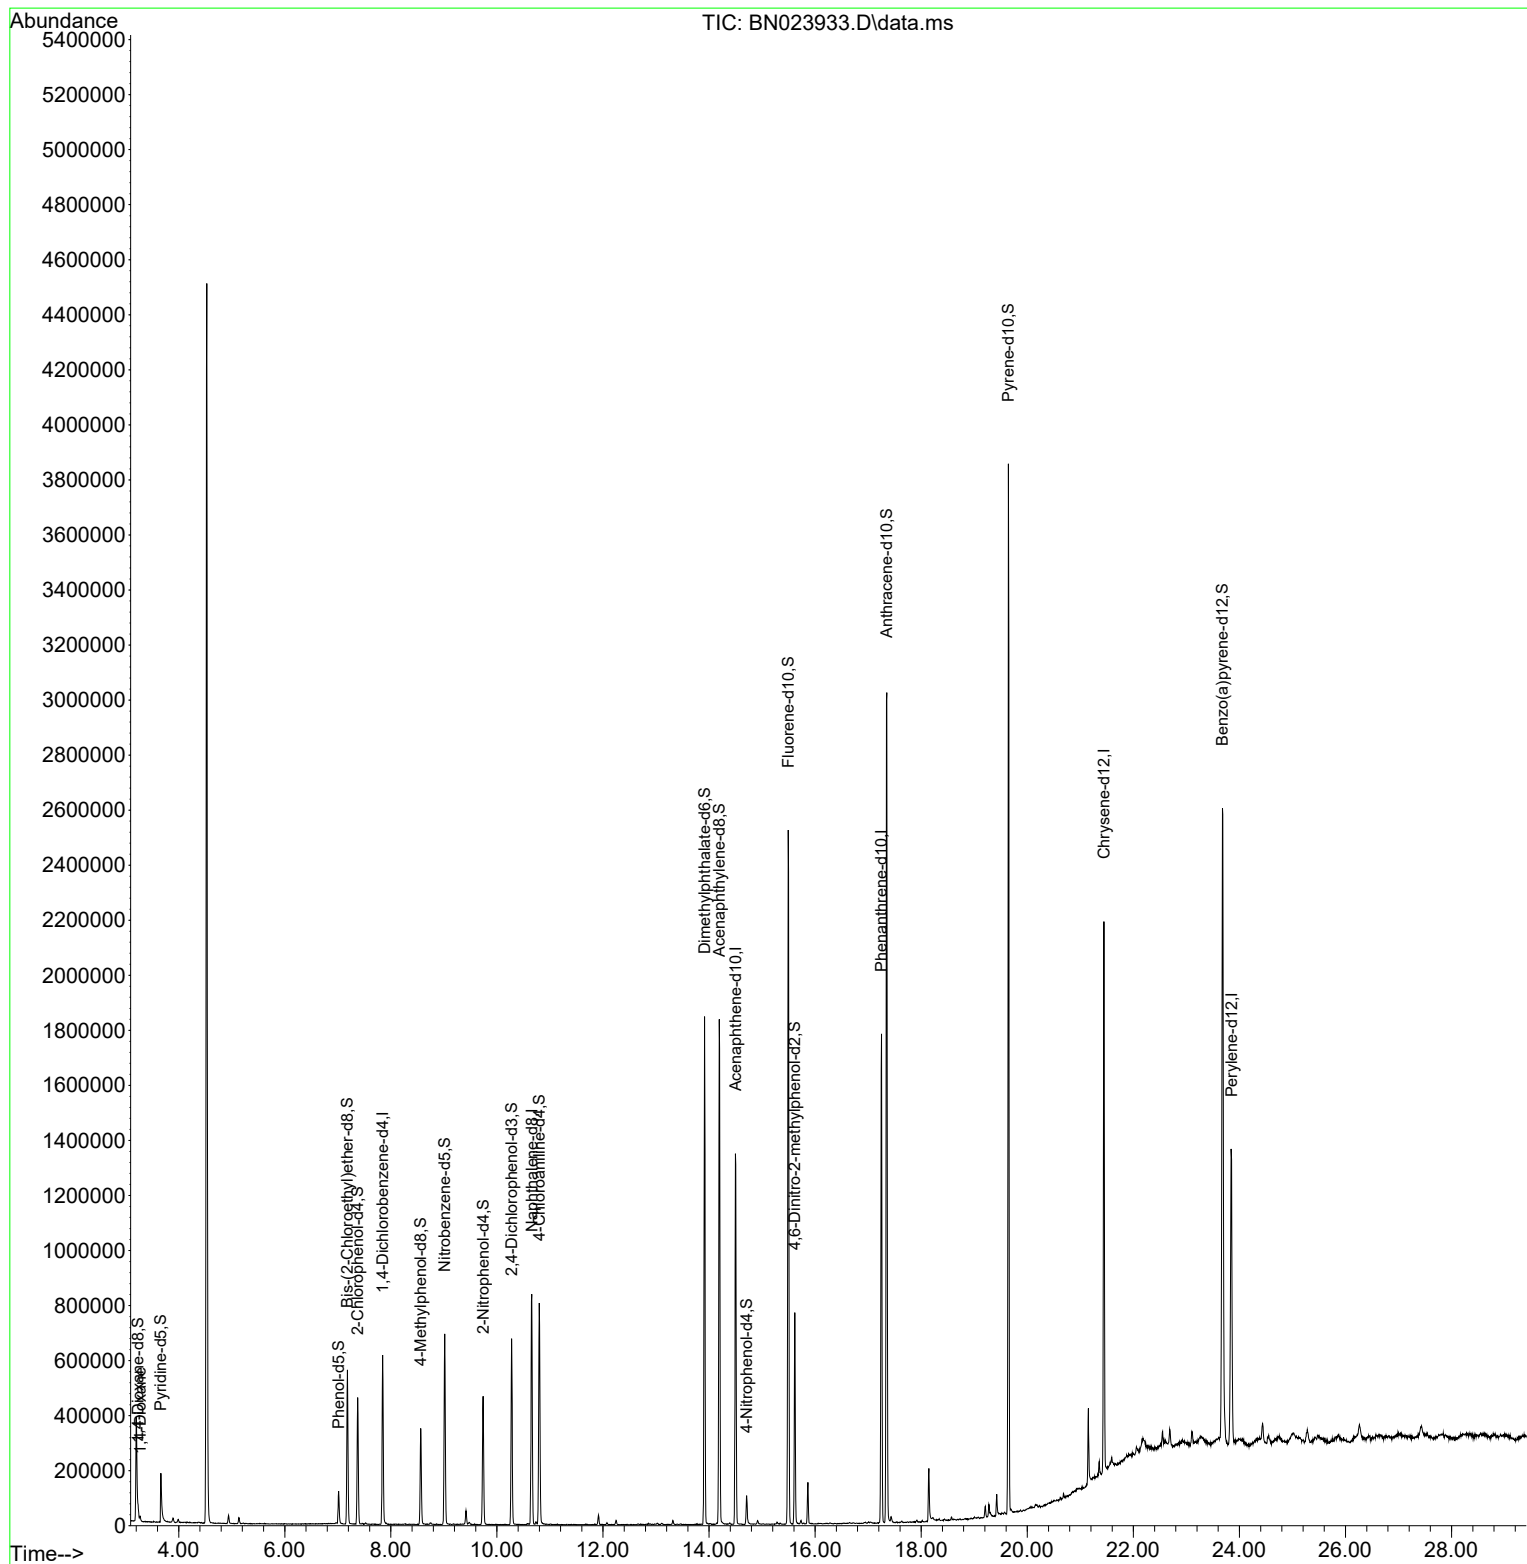

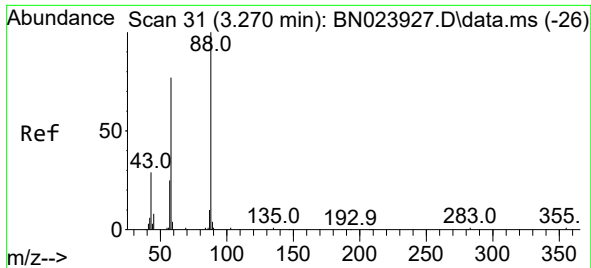

#2
 1,4-Dioxane
 Concen: 2.331 ng/uL
 RT: 3.276 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN023933.D
 Acq: 03 Feb 2023 09:02

Instrument :
 BNA_N
 ClientSampleId :
 C0LC9

Tgt Ion: 88 Resp: 8995
 Ion Ratio Lower Upper
 88 100
 43 34.7 42.1 63.1#
 58 58.2 53.8 80.6

