

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023937.D
 Acq On : 03 Feb 2023 11:29
 Operator : CG/JU
 Sample : 01295-01DL 2X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC4DL

Quant Time: Feb 03 21:50:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	162294	20.000	ng/u1	0.00
20) Naphthalene-d8	10.658	136	676892	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	464235	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	1035085	20.000	ng/u1	0.00
79) Chrysene-d12	21.445	240	886766	20.000	ng/u1	0.00
88) Perylene-d12	23.845	264	829921	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	10271	2.554	ng/uL	0.00
4) Pyridine-d5	3.664	84	56289	5.010	ng/u1	0.00
7) Phenol-d5	7.017	99	45911	3.239	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	148853	16.619	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	136204	12.291	ng/u1	0.00
15) 4-Methylphenol-d8	8.564	113	86511	7.695	ng/u1	-0.01
21) Nitrobenzene-d5	9.016	128	85826	15.628	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	90894	14.546	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	164855	14.129	ng/u1	0.00
31) 4-Chloroaniline-d4	10.799	131	218508	13.727	ng/u1	-0.01
46) Dimethylphthalate-d6	13.916	166	712939	19.236	ng/u1	0.00
49) Acenaphthylene-d8	14.193	160	680141	16.964	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	15599	2.321	ng/u1	0.00
60) Fluorene-d10	15.493	176	593821	19.111	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	97329	13.288	ng/u1	0.00
73) Anthracene-d10	17.345	188	978925	20.314	ng/u1	0.00
81) Pyrene-d10	19.645	212	1165229	21.643	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	911798	21.168	ng/u1	-0.01


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.270	88	74105	17.891	ng/uL#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023937.D
Acq On : 03 Feb 2023 11:29
Operator : CG/JU
Sample : 01295-01DL 2X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC4DL

Quant Time: Feb 03 21:50:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

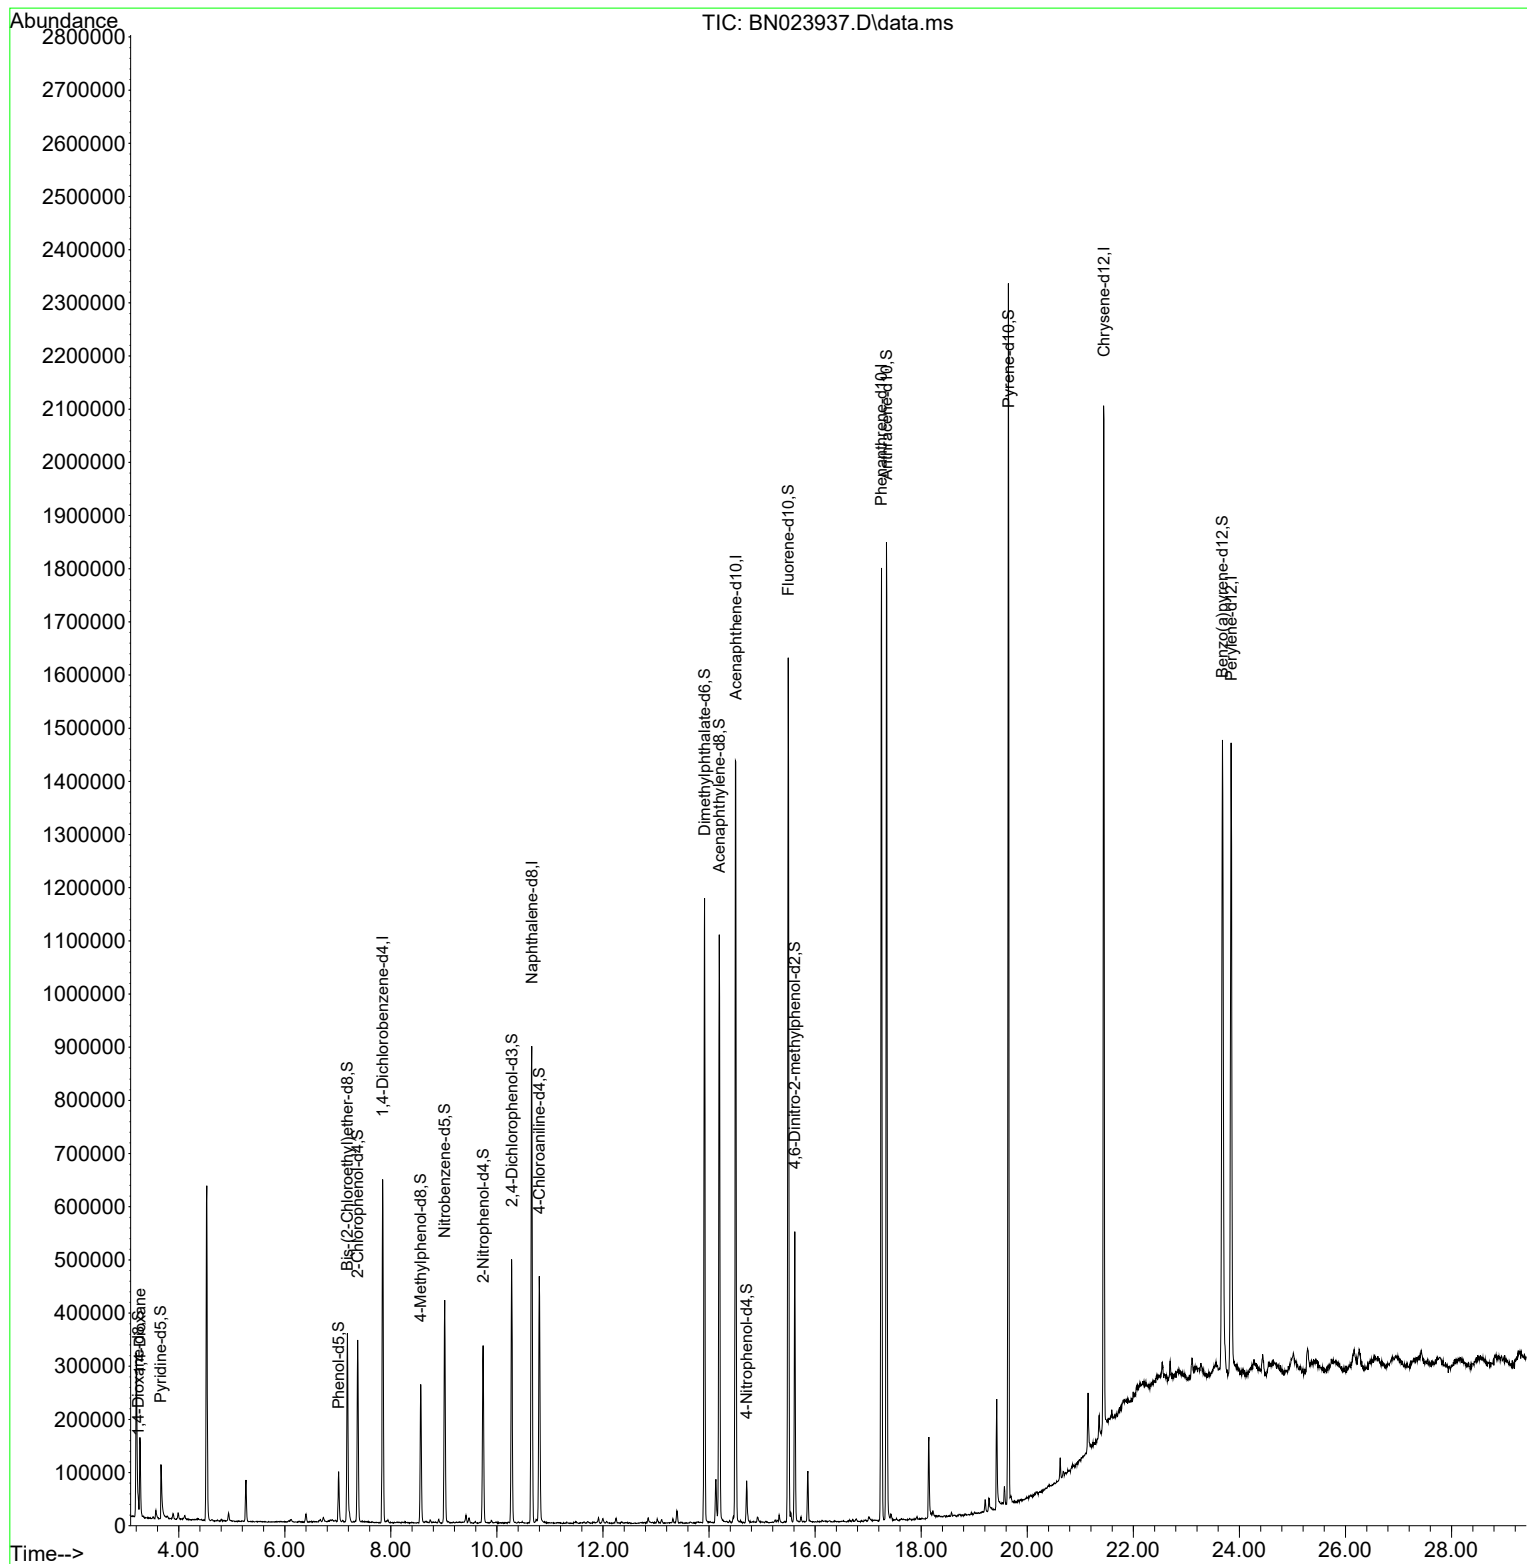

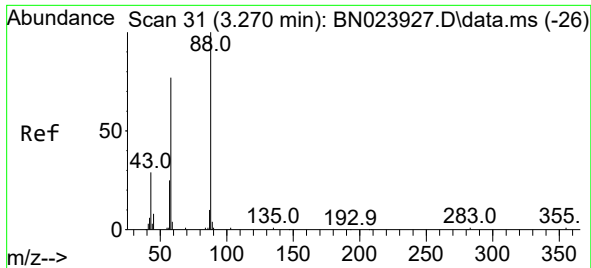

#2
 1,4-Dioxane
 Concen: 17.891 ng/uL
 RT: 3.270 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN023937.D
 Acq: 03 Feb 2023 11:29

Instrument :
 BNA_N
 ClientSampleId :
 C0LC4DL

Tgt Ion: 88 Resp: 74105
 Ion Ratio Lower Upper
 88 100
 43 29.3 42.1 63.1#
 58 66.2 53.8 80.6

