

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023943.D
 Acq On : 03 Feb 2023 15:10
 Operator : CG/JU
 Sample : 01316-06
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44H0

Quant Time: Feb 03 21:52:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	149738	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	628120	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	426336	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	942456	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	777465	20.000	ng/u1	-0.02
88) Perylene-d12	23.815	264	720790	20.000	ng/u1	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	15649	4.218	ng/uL	0.00
4) Pyridine-d5	3.663	84	97666	9.422	ng/u1	0.00
7) Phenol-d5	7.016	99	85762	6.559	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	263321	31.865	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	253465	24.791	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	168498	16.244	ng/u1	-0.01
21) Nitrobenzene-d5	9.016	128	165744	32.523	ng/u1	0.00
24) 2-Nitrophenol-d4	9.739	143	181054	31.224	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	326591	30.164	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	325560	22.041	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	1321238	38.817	ng/u1	0.00
49) Acenaphthylene-d8	14.192	160	1273803	34.595	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	37076	6.008	ng/u1	0.00
60) Fluorene-d10	15.492	176	1057300	37.053	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	211624	31.732	ng/u1	0.00
73) Anthracene-d10	17.351	188	1764453	40.214	ng/u1	0.00
81) Pyrene-d10	19.645	212	1984449	42.042	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.668	264	1599684	42.760	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.045	94	35998	2.739	ng/u1	99
59) Diethylphthalate	15.321	149	242068	7.212	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023943.D
Acq On : 03 Feb 2023 15:10
Operator : CG/JU
Sample : 01316-06
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44H0

Quant Time: Feb 03 21:52:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration




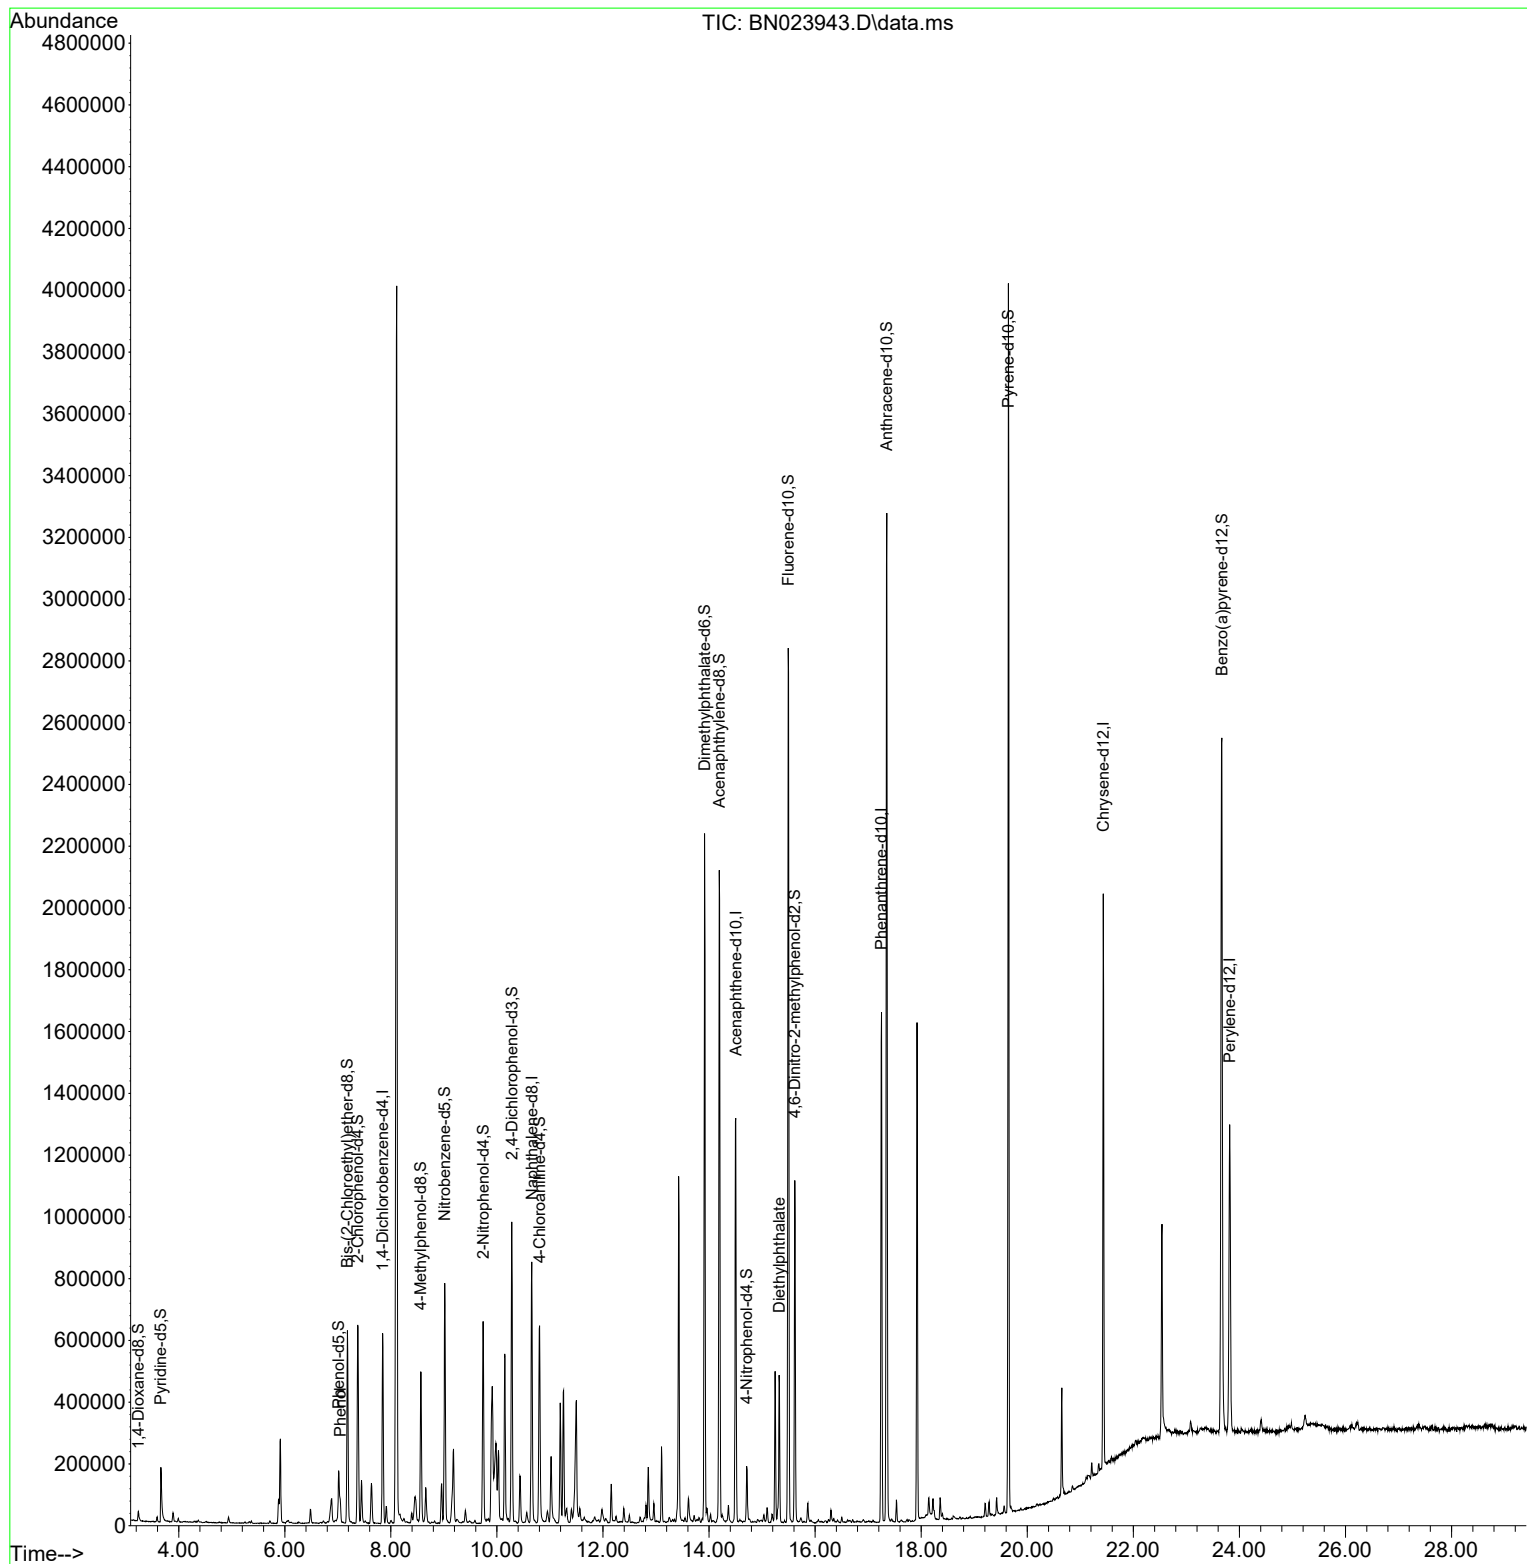


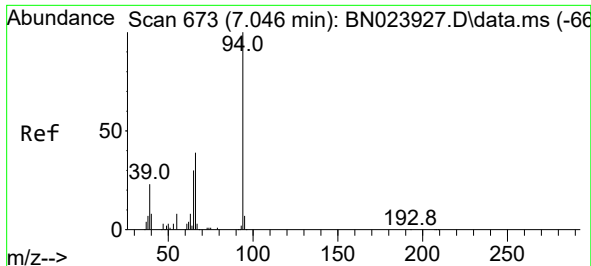

#8
Phenol
Concen: 2.739 ng/ul
RT: 7.045 min Scan# 61
Delta R.T. -0.006 min
Lab File: BN023943.D
Acq: 03 Feb 2023 15:10

Instrument :
BNA_N
ClientSampleId :
A44H0

Tgt Ion: 94 Resp: 35998
Ion Ratio Lower Upper
94 100
65 31.2 24.1 36.1
66 41.0 32.4 48.6

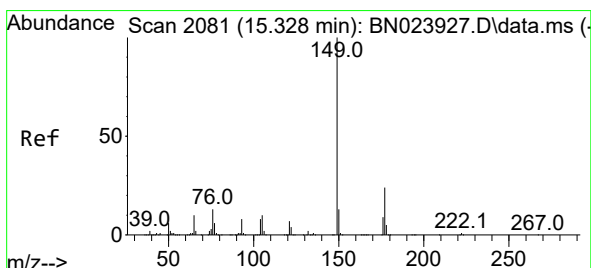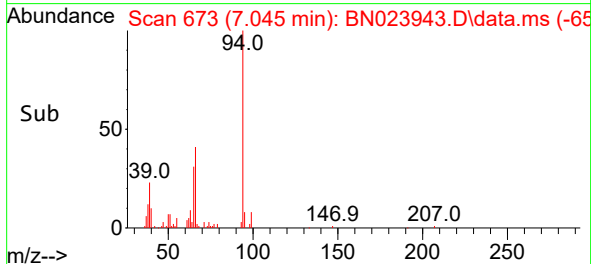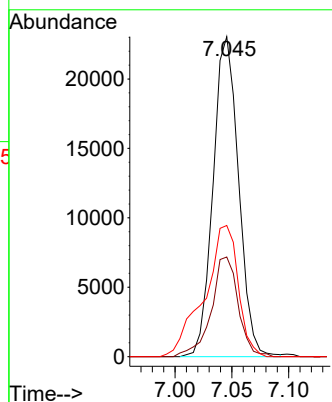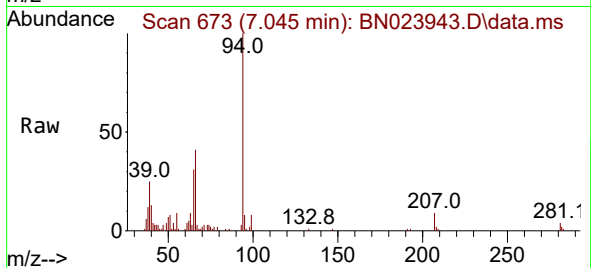

#59
Diethylphthalate
Concen: 7.212 ng/ul
RT: 15.321 min Scan# 2080
Delta R.T. -0.012 min
Lab File: BN023943.D
Acq: 03 Feb 2023 15:10

Tgt Ion: 149 Resp: 242068
Ion Ratio Lower Upper
149 100
177 22.2 17.8 26.6
150 13.0 9.4 14.2

