




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023907.D
Acq On : 02 Feb 2023 16:26
Operator : CG/JU
Sample : 01362-12DL 30X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4488DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:18:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

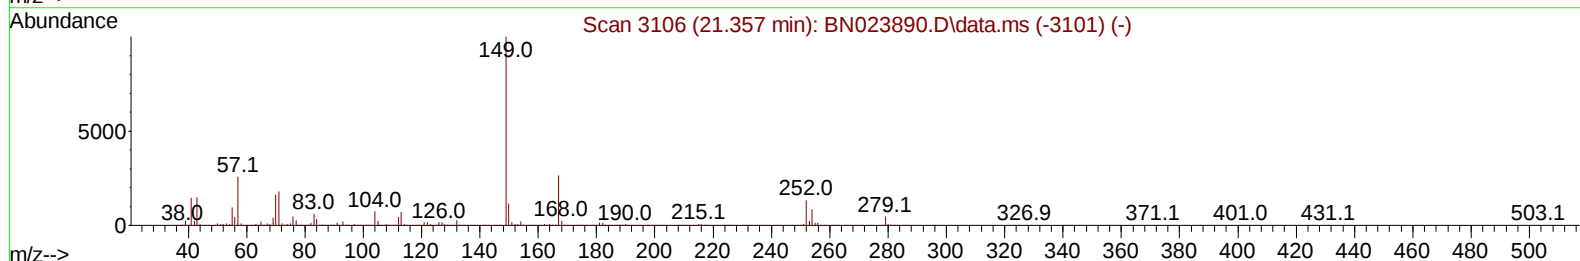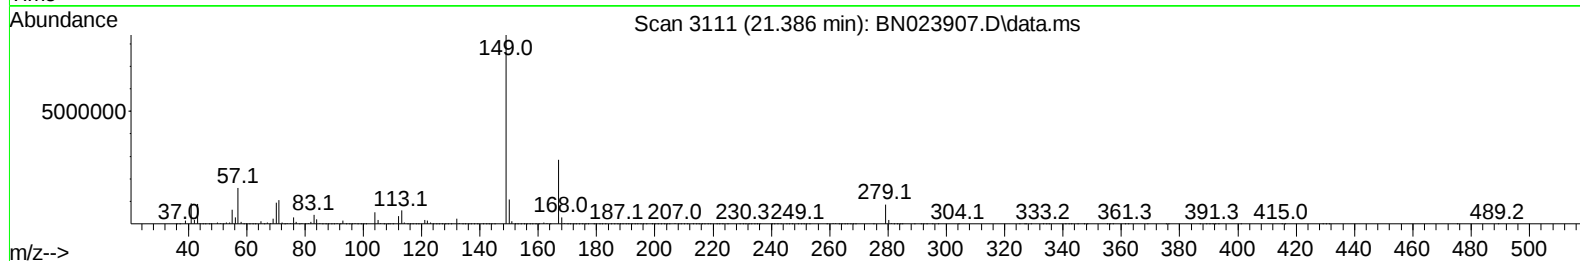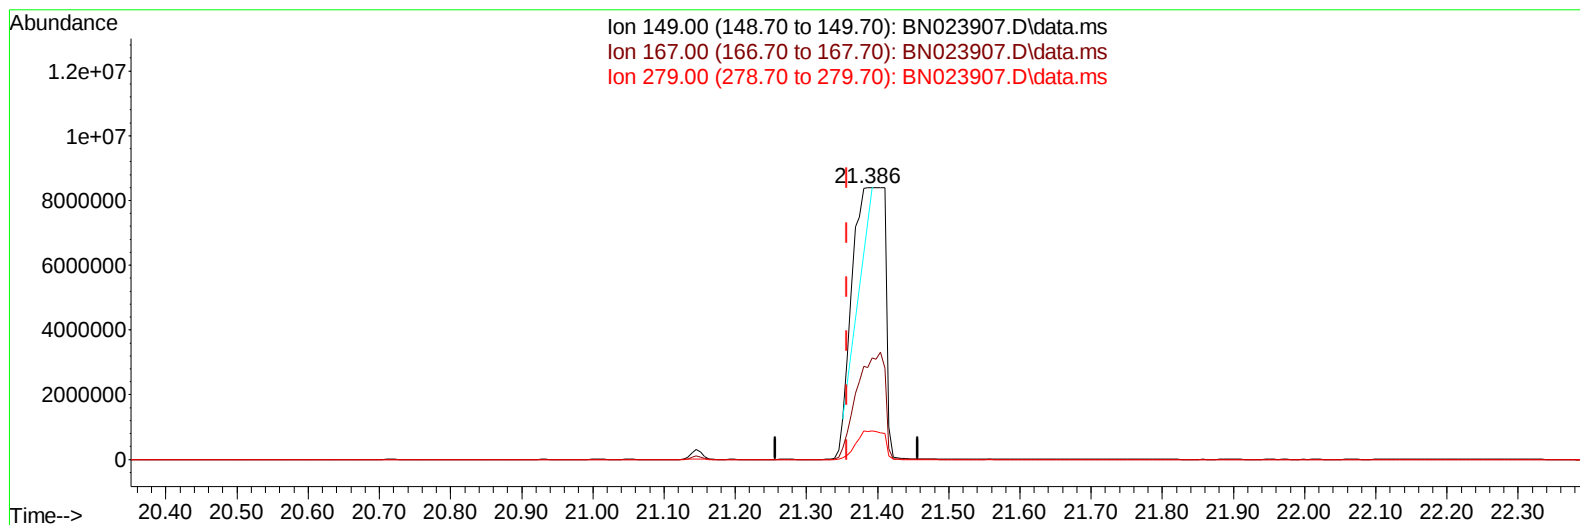

TIC: BN023907.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.386min (+ 0.029) 175.32 ng/u1

response 5492802

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	26.50	33.88#
279.00	4.70	10.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023907.D
Acq On : 02 Feb 2023 16:26
Operator : CG/JU
Sample : 01362-12DL 30X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4488DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:18:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

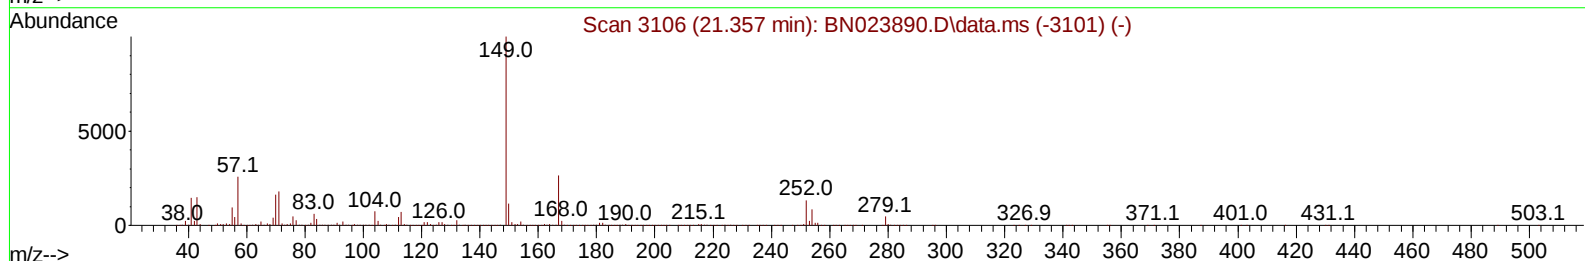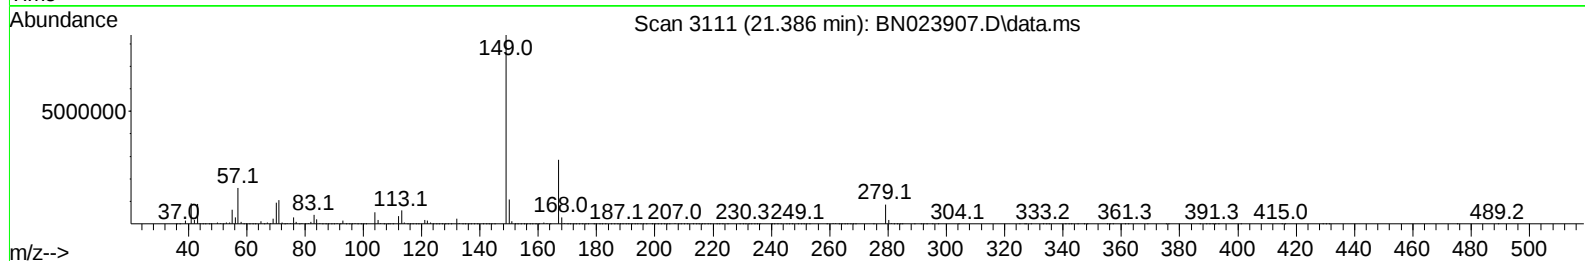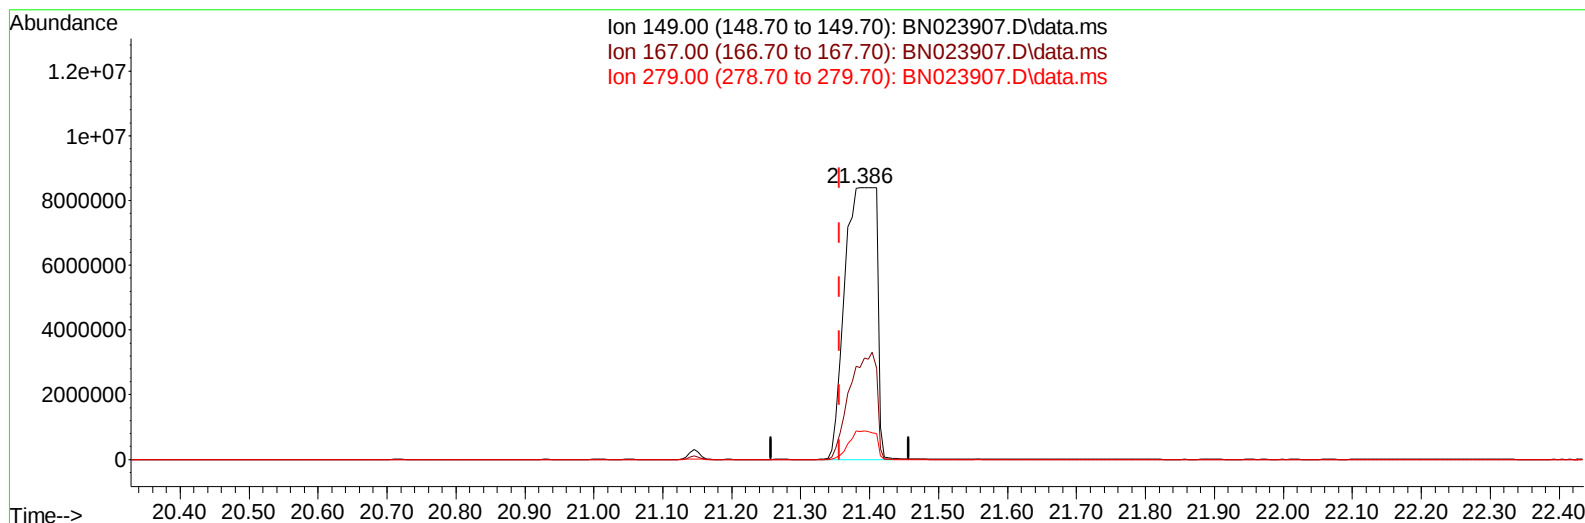

TIC: BN023907.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.386min (+ 0.029) 856.21 ng/ul m

response 26824705

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	26.50	33.88#
279.00	4.70	10.20#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023907.D
 Acq On : 02 Feb 2023 16:26
 Operator : CG/JU
 Sample : 01362-12DL 30X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4488DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
 Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:18:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.852	152		159006	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136		658850	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164		427370	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188		907806	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240		706309	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264		704807	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.022	99		12471	0.898	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67		8360	0.953	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132		10384	0.956	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113		10147	0.921	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128		4360	0.816	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143		4697	0.772	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165		9817	0.864	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131		12950	0.836	ng/ul	0.00
46) Dimethylphthalate-d6	13.916	166		33902	0.994	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160		30329	0.822	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.498	176		29875	1.044	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.351	188		40703	0.963	ng/ul	0.00
81) Pyrene-d10	19.645	212		48867	1.140	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264		37468	1.024	ng/ul	0.00
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.386	149		26824705m	856.213	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023907.D
Acq On : 02 Feb 2023 16:26
Operator : CG/JU
Sample : 01362-12DL 30X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4488DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 02/03/2023
Supervised By :Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:18:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

