

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023898.D
 Acq On : 02 Feb 2023 10:32
 Operator : CG/JU
 Sample : 01362-16
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4494

Quant Time: Feb 02 14:04:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.852	152	144771	20.000 ng/u1	0.00
20) Naphthalene-d8	10.663	136	588378	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.504	164	368250	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.251	188	765284	20.000 ng/u1	0.00
79) Chrysene-d12	21.451	240	659276	20.000 ng/u1	0.00
88) Perylene-d12	23.851	264	725027	20.000 ng/u1	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.240	96	12816	3.573 ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000 ng/u1	
7) Phenol-d5	7.028	99	275410	21.785 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	171675	21.487 ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	216479	21.900 ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	207733	20.714 ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	105327	22.064 ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	119807	22.057 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	223223	22.009 ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	258658	18.694 ng/u1	0.00
46) Dimethylphthalate-d6	13.922	166	797609	27.129 ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	789700	24.830 ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	136294	25.570 ng/u1	0.00
60) Fluorene-d10	15.498	176	680873	27.625 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	126610	23.380 ng/u1	0.00
73) Anthracene-d10	17.351	188	1162205	32.620 ng/u1	0.00
81) Pyrene-d10	19.651	212	1348622	33.693 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.686	264	1254390	33.335 ng/u1	0.00
Target Compounds					
86) Bis(2-ethylhexyl)phtha...	21.357	149	1585112	54.204 ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023898.D
Acq On : 02 Feb 2023 10:32
Operator : CG/JU
Sample : 01362-16
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4494

Quant Time: Feb 02 14:04:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

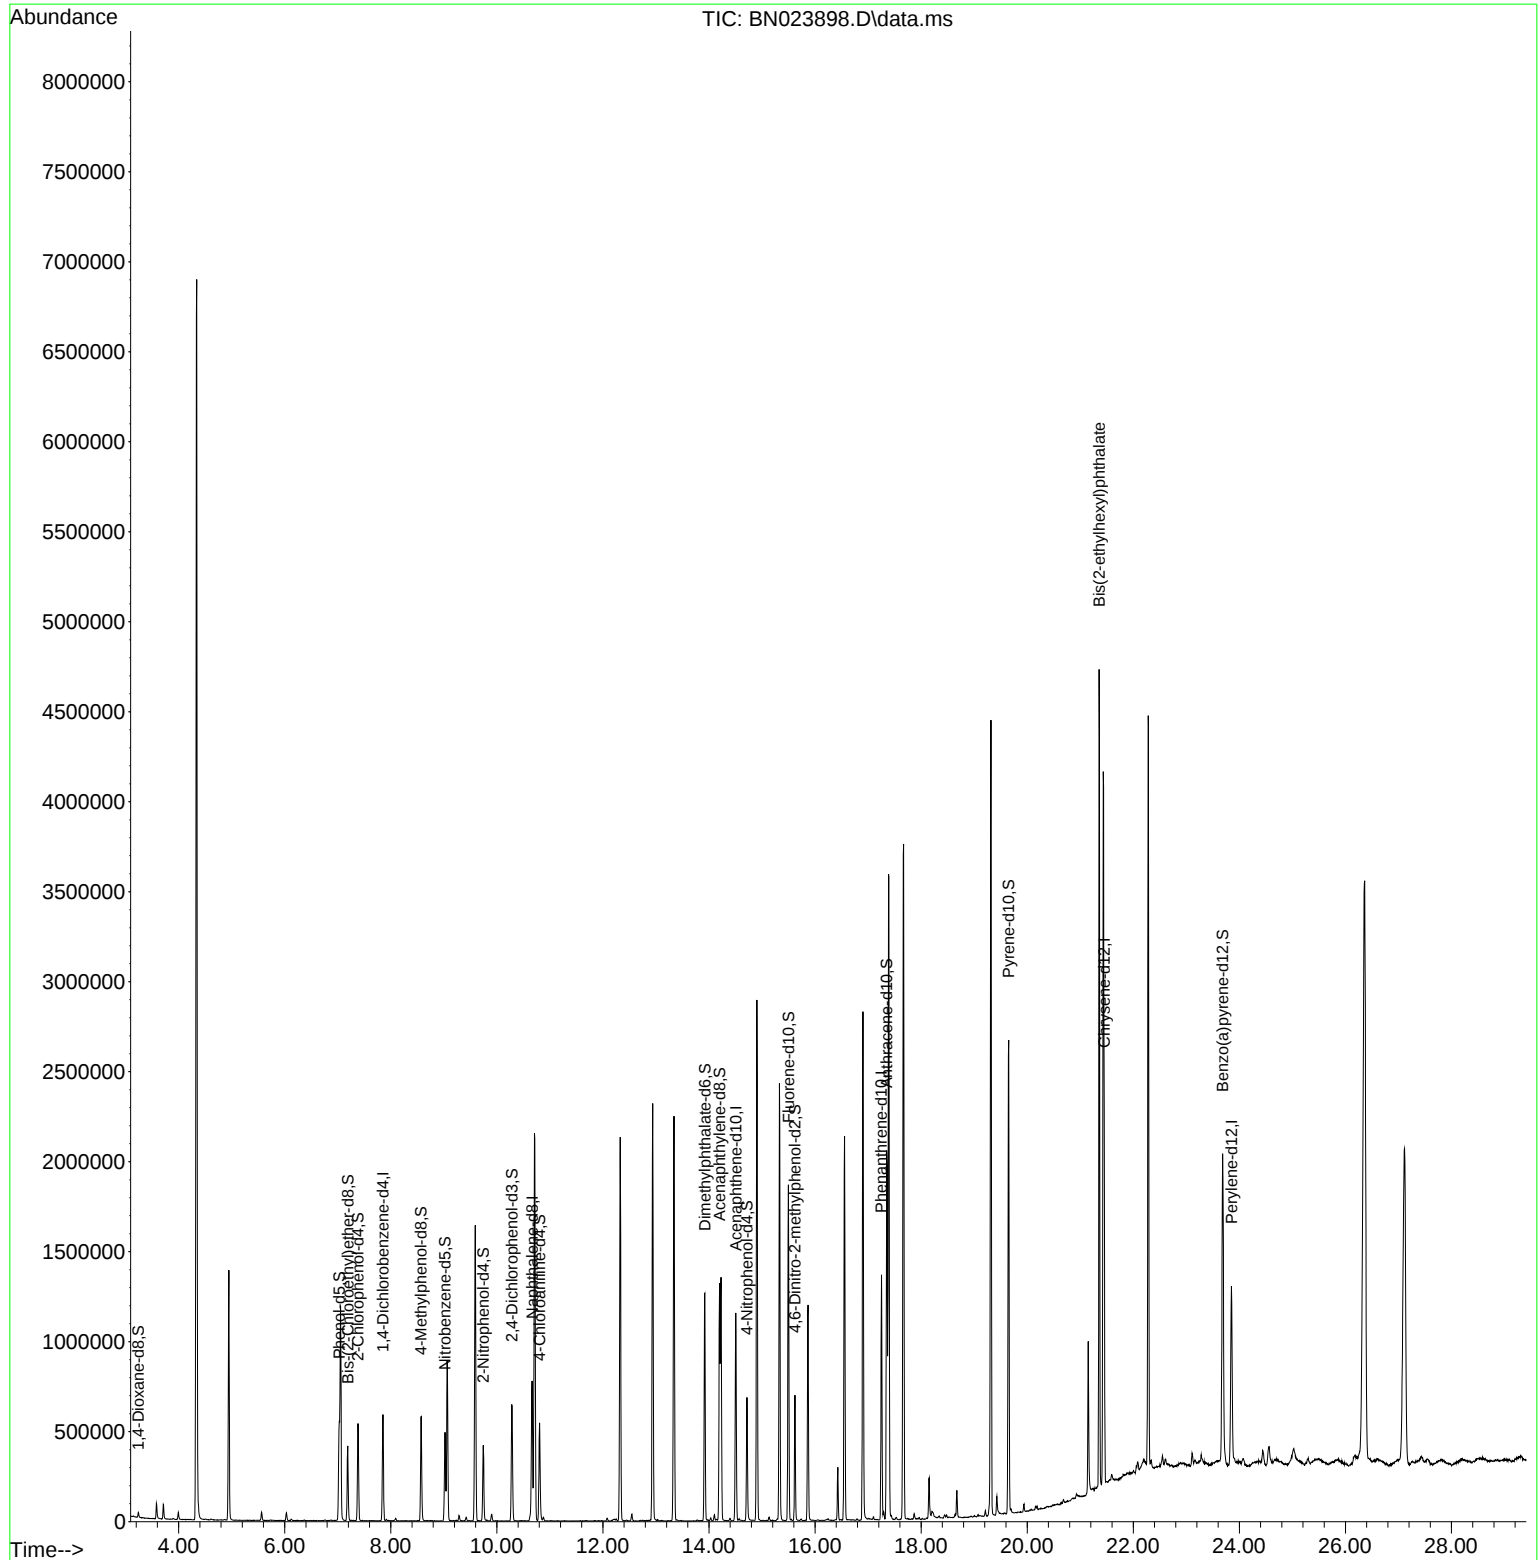

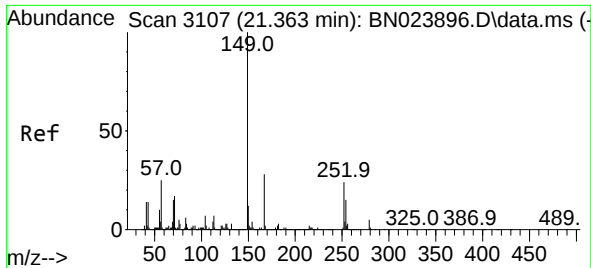

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 54.204 ng/ul
 RT: 21.357 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN023898.D
 Acq: 02 Feb 2023 10:32

Instrument :
 BNA_N
 ClientSampleId :
 A4494

Tgt Ion:149 Resp: 1585112
 Ion Ratio Lower Upper
 149 100
 167 27.1 21.2 31.8
 279 4.5 3.8 5.6

