

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023900.D
 Acq On : 02 Feb 2023 12:10
 Operator : CG/JU
 Sample : 01362-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4488

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 02/03/2023
 Supervised By : Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:16:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	178800	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	642338	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	373224	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	772657m	20.000	ng/u1	0.04
79) Chrysene-d12	21.451	240	35497m	20.000	ng/u1	0.00
88) Perylene-d12	23.874	264	748591	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	22358	5.047	ng/uL	0.00
4) Pyridine-d5	3.664	84	297604	24.043	ng/u1	0.00
7) Phenol-d5	7.022	99	405997	26.002	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	264239	26.778	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	330432	27.066	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	303310	24.488	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	151405	29.052	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	168196	28.364	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	291089	26.290	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	370450	24.525	ng/u1	0.00
46) Dimethylphthalate-d6	13.922	166	715713	24.019	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	888790	27.574	ng/u1	0.00
54) 4-Nitrophenol-d4	14.851	143	111174m	20.579	ng/u1	0.14
60) Fluorene-d10	15.504	176	902188m	36.116	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	51895m	9.492	ng/u1	0.15
73) Anthracene-d10	17.381	188	709006	19.710	ng/u1	0.03
81) Pyrene-d10	19.663	212	1069209m	496.124	ng/u1	0.02
92) Benzo(a)pyrene-d12	23.733	264	1084628	27.916	ng/u1	0.04

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.392	149	116642582m	74081.017	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023900.D
Acq On : 02 Feb 2023 12:10
Operator : CG/JU
Sample : 01362-12
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4488

Quant Time: Feb 03 01:16:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 02/03/2023
Supervised By : Jagrut Upadhyay 02/03/2023

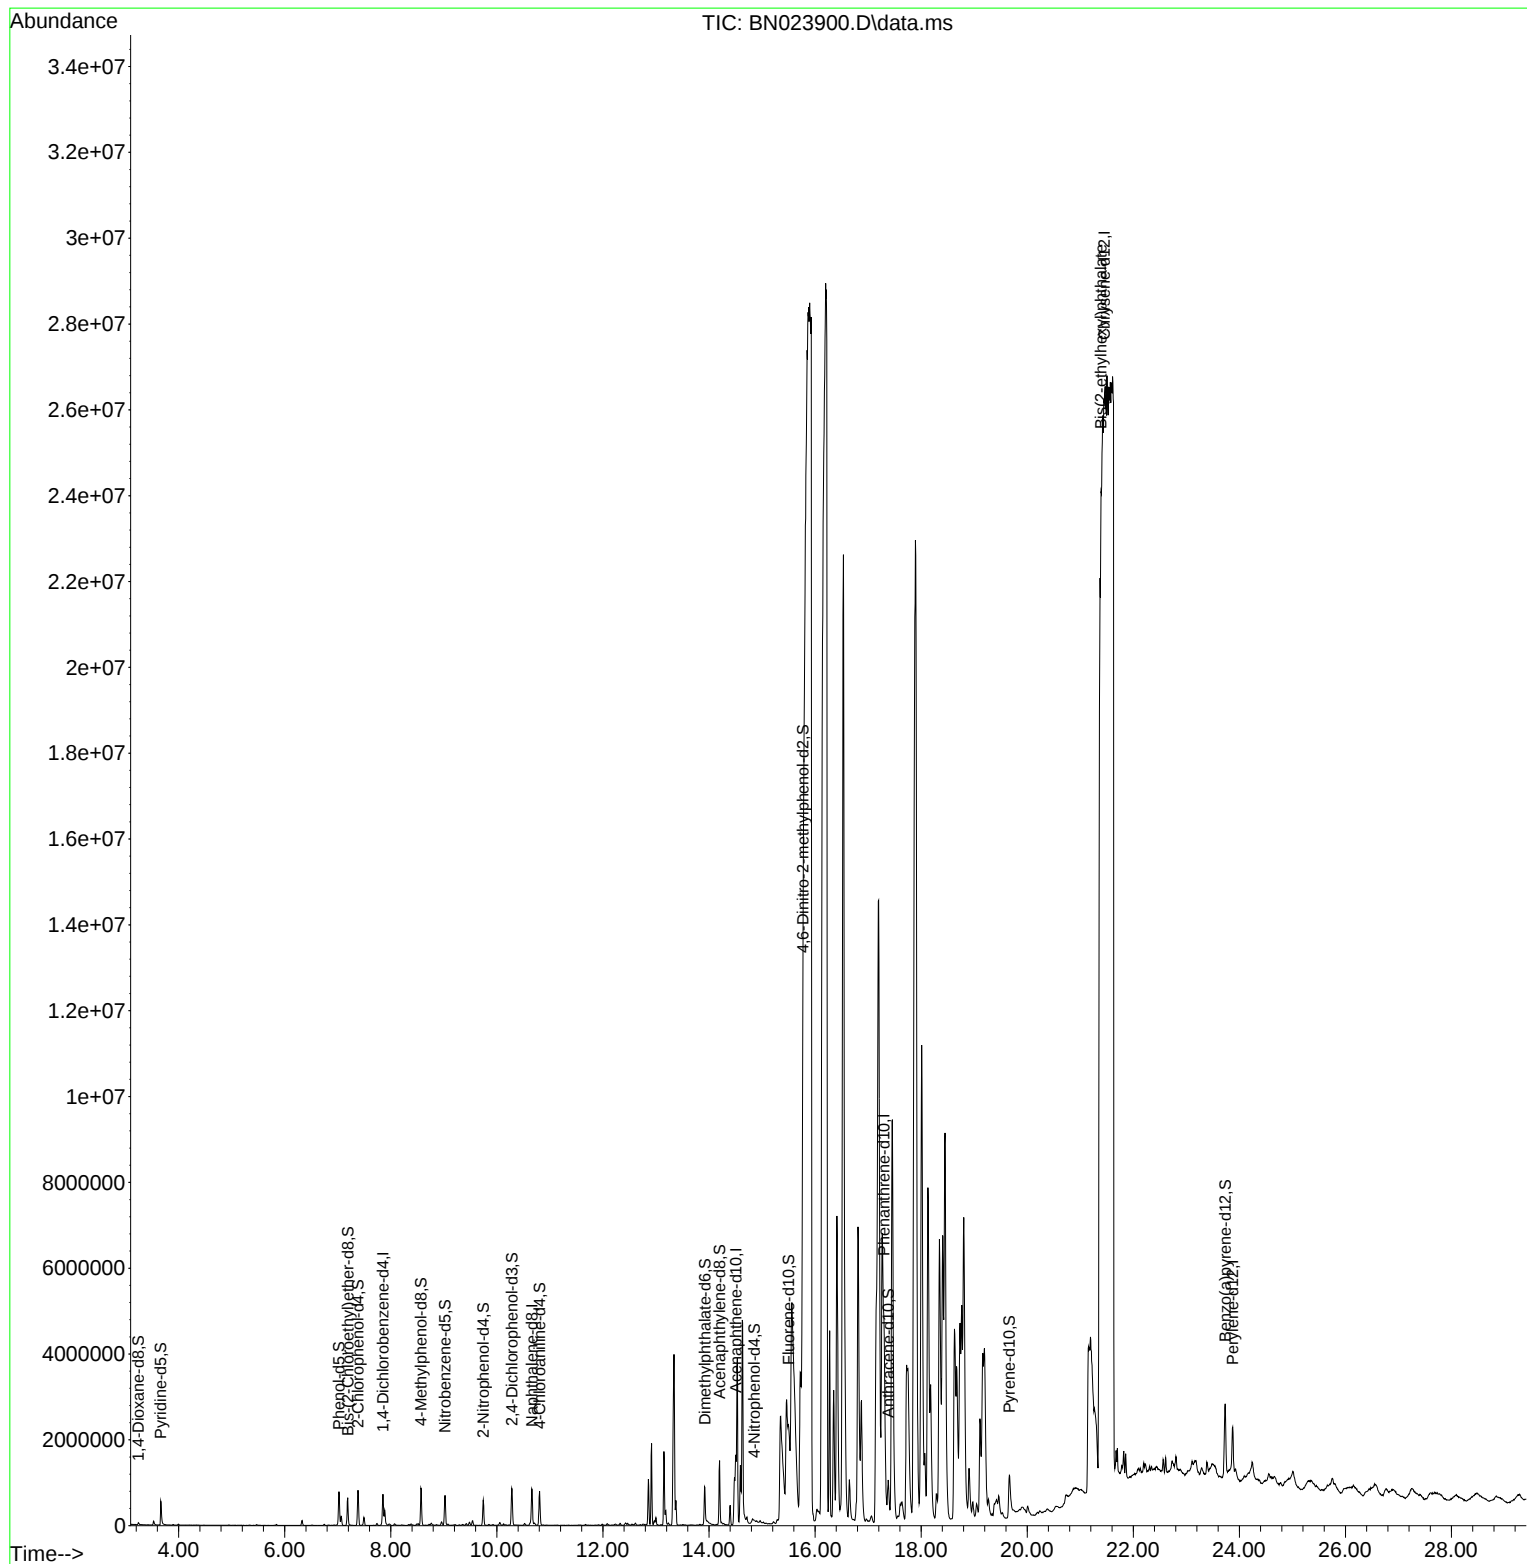

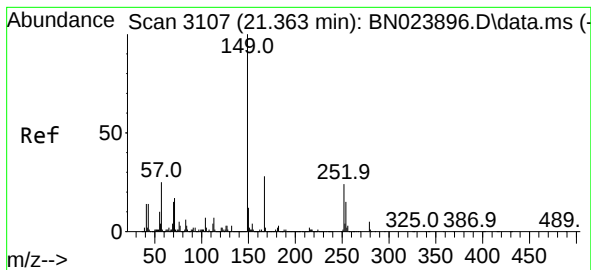

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 74081.017 ng/ul m
 RT: 21.392 min Scan# 3112
 Delta R.T. 0.035 min
 Lab File: BN023900.D
 Acq: 02 Feb 2023 12:10

Instrument :
 BNA_N
 ClientSampleId :
 A4488

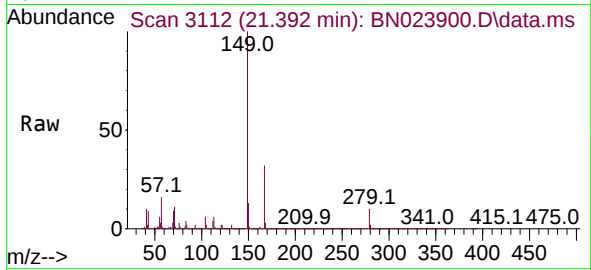

Tgt Ion:149 Resp:11664258
 Ion Ratio Lower Upper
 149 100
 167 31.8 21.2 31.8
 279 9.6 3.8 5.6

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 02/03/2023
 Supervised By :Jagrut Upadhyay 02/03/2023

