

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023904.D
 Acq On : 02 Feb 2023 14:36
 Operator : CG/JU
 Sample : 01362-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4443

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 02/03/2023
 Supervised By : Jagrut Upadhyay 02/03/2023

Quant Time: Feb 03 01:18:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	159125	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	663600	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	427615	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.322	188	1736826m	20.000	ng/u1	0.06
79) Chrysene-d12	21.445	240	578911	20.000	ng/u1	0.00
88) Perylene-d12	23.839	264	648087	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	7381	1.872	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.022	99	158892	11.435	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	107117	12.198	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	134473	12.377	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	141025	12.794	ng/u1	0.00
21) Nitrobenzene-d5	9.022	128	71964	13.366	ng/u1	0.00
24) 2-Nitrophenol-d4	9.746	143	85744	13.996	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	155066	13.556	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	172525	11.056	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	506074	14.824	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	568959	15.406	ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	62087	10.031	ng/u1	0.00
60) Fluorene-d10	15.498	176	437910	15.301	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	49987	4.067	ng/u1	0.02
73) Anthracene-d10	17.410	188	617128m	7.632	ng/u1	0.06
81) Pyrene-d10	19.663	212	641569	18.254	ng/u1	0.02
92) Benzo(a)pyrene-d12	23.680	264	518214	15.406	ng/u1	-0.01

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.386	149	37465811m	1459.032	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023904.D
Acq On : 02 Feb 2023 14:36
Operator : CG/JU
Sample : 01362-05
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4443

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 02/03/2023
Supervised By : Jagrut Upadhyay 02/03/2023


Quant Time: Feb 03 01:18:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

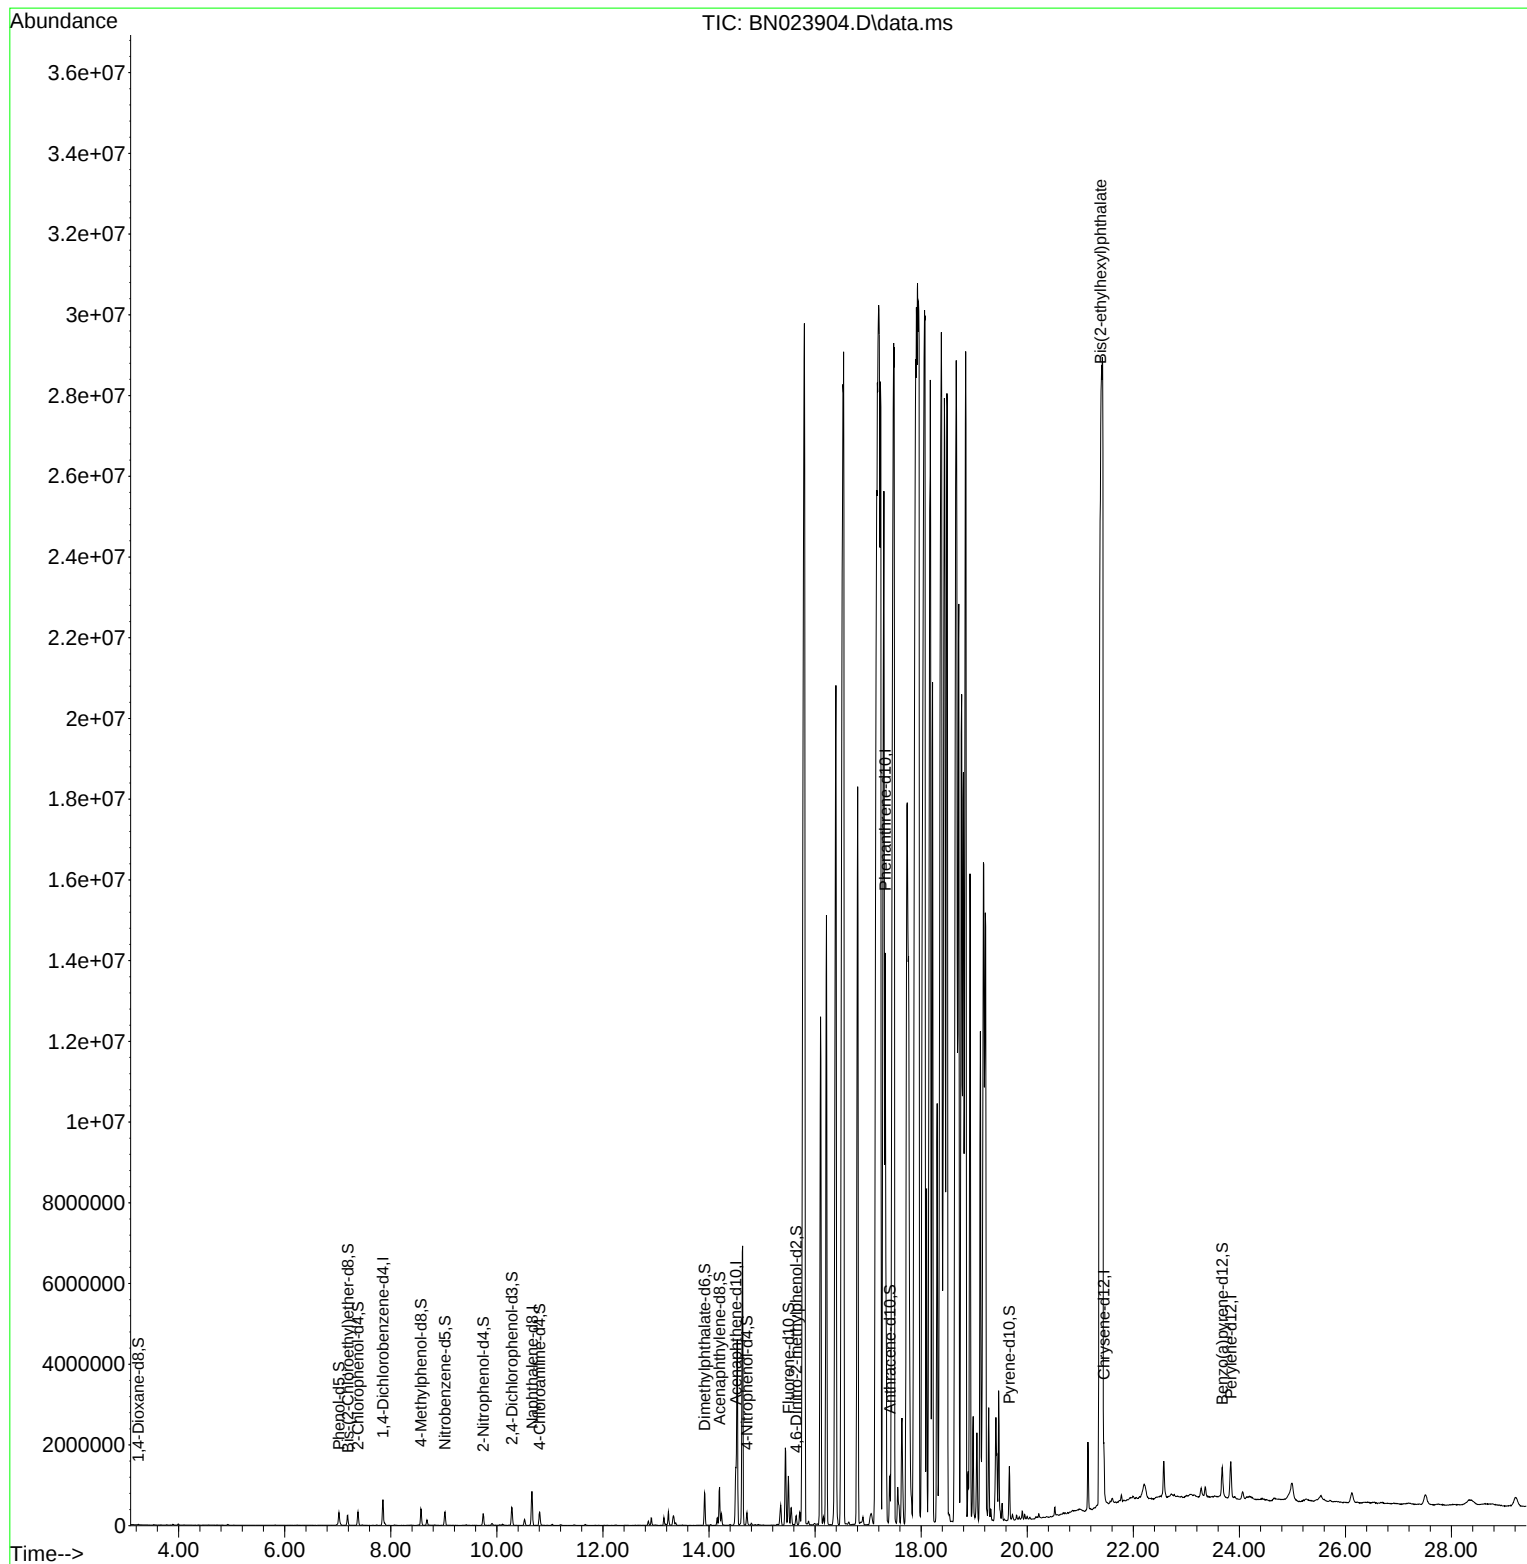

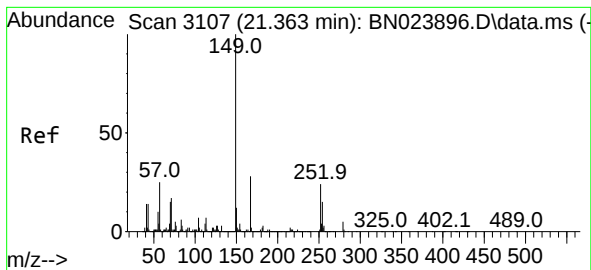

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1459.032 ng/ul m
 RT: 21.386 min Scan# 3111
 Delta R.T. 0.029 min
 Lab File: BN023904.D
 Acq: 02 Feb 2023 14:36

Instrument :
 BNA_N
 ClientSampleId :
 A4443

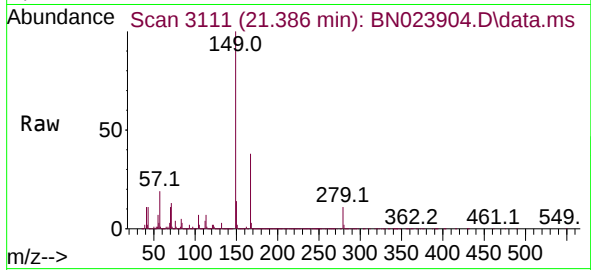

Tgt Ion:149 Resp:37465811
 Ion Ratio Lower Upper
 149 100
 167 38.2 21.2 31.8
 279 10.7 3.8 5.6

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 02/03/2023
 Supervised By :Jagrut Upadhyay 02/03/2023

