

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023923.D
 Acq On : 03 Feb 2023 02:20
 Operator : CG/JU
 Sample : 01295-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC4

Quant Time: Feb 03 04:34:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	157325	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	658002	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	436128	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	982049	20.000	ng/u1	0.00
79) Chrysene-d12	21.439	240	879772	20.000	ng/u1	-0.01
88) Perylene-d12	23.827	264	852502	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	17930	4.600	ng/uL	0.00
4) Pyridine-d5	3.664	84	112119	10.294	ng/u1	0.00
7) Phenol-d5	7.016	99	84001	6.114	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	261332	30.099	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	249082	23.187	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	164517	15.096	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	159777	29.928	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	169177	27.851	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	305497	26.934	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	403342	26.066	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	1241722	35.662	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	1248326	33.142	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	34098	5.401	ng/u1	0.00
60) Fluorene-d10	15.498	176	1052765	36.066	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	190763	27.451	ng/u1	0.00
73) Anthracene-d10	17.351	188	1767625	38.662	ng/u1	0.00
81) Pyrene-d10	19.645	212	2055138	38.476	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.674	264	1640494	37.076	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.275	88	129074	32.146	ng/uL#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023923.D
Acq On : 03 Feb 2023 02:20
Operator : CG/JU
Sample : 01295-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC4


Quant Time: Feb 03 04:34:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

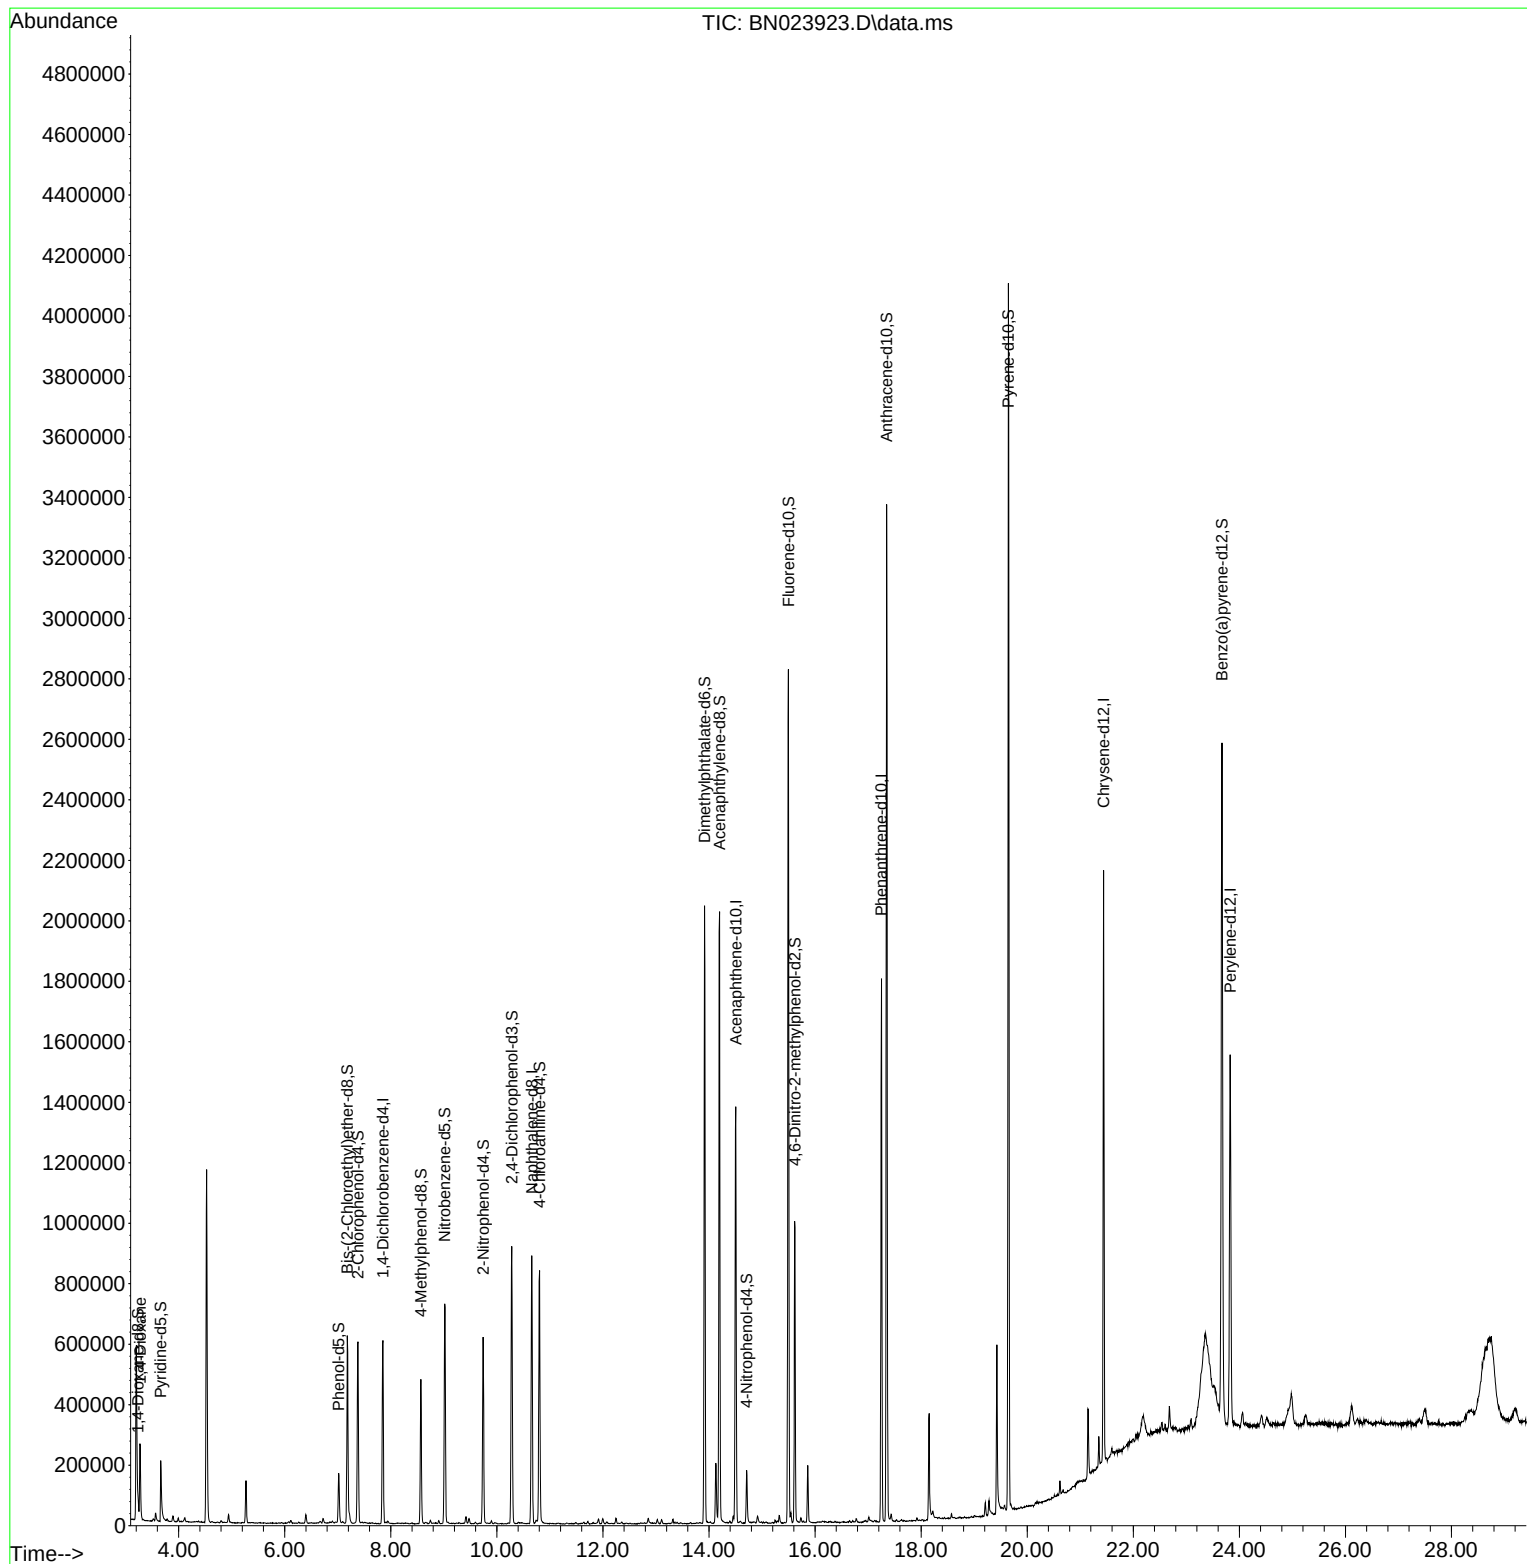

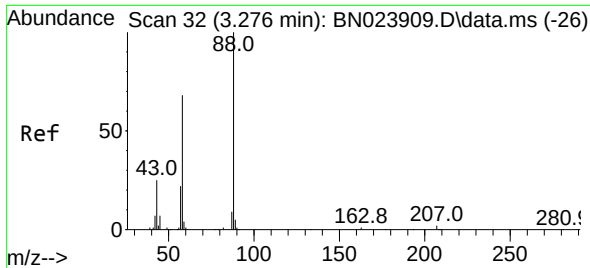

#2
 1,4-Dioxane
 Concen: 32.146 ng/uL
 RT: 3.275 min Scan# 31
 Delta R.T. -0.001 min
 Lab File: BN023923.D
 Acq: 03 Feb 2023 02:20

Instrument :
 BNA_N
 ClientSampleId :
 C0LC4

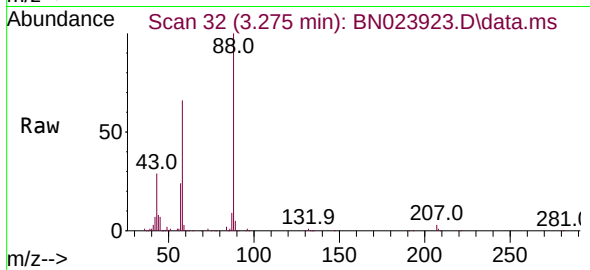

Tgt Ion: 88 Resp: 129074
 Ion Ratio Lower Upper
 88 100
 43 28.6 42.1 63.1#
 58 66.5 53.8 80.6

