

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023925.D
 Acq On : 03 Feb 2023 03:33
 Operator : CG/JU
 Sample : 01295-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC6

Quant Time: Feb 03 04:38:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 02 02:10:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	152611	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	641443	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	429449	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.251	188	993670	20.000	ng/u1	0.00
79) Chrysene-d12	21.439	240	984858	20.000	ng/u1	-0.01
88) Perylene-d12	23.839	264	976865	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	16753	4.431	ng/uL	0.00
4) Pyridine-d5	3.664	84	101387	9.597	ng/u1	0.00
7) Phenol-d5	7.016	99	65987	4.951	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	234451	27.837	ng/u1	0.00
11) 2-Chlorophenol-d4	7.375	132	186481	17.896	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	123018	11.636	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	140744	27.044	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	124637	21.048	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	216814	19.609	ng/u1	0.00
31) 4-Chloroaniline-d4	10.804	131	334416	22.170	ng/u1	0.00
46) Dimethylphthalate-d6	13.916	166	1031662	30.090	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	1063923	28.686	ng/u1	0.00
54) 4-Nitrophenol-d4	14.710	143	26916	4.330	ng/u1	0.00
60) Fluorene-d10	15.498	176	916429	31.883	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.616	200	151703	21.575	ng/u1	0.00
73) Anthracene-d10	17.351	188	1674849	36.205	ng/u1	0.00
81) Pyrene-d10	19.645	212	2029564	33.943	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1854337	36.574	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.275	88	8473	2.175	ng/uL#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023925.D
Acq On : 03 Feb 2023 03:33
Operator : CG/JU
Sample : 01295-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC6

Quant Time: Feb 03 04:38:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 02 02:10:45 2023
Response via : Initial Calibration

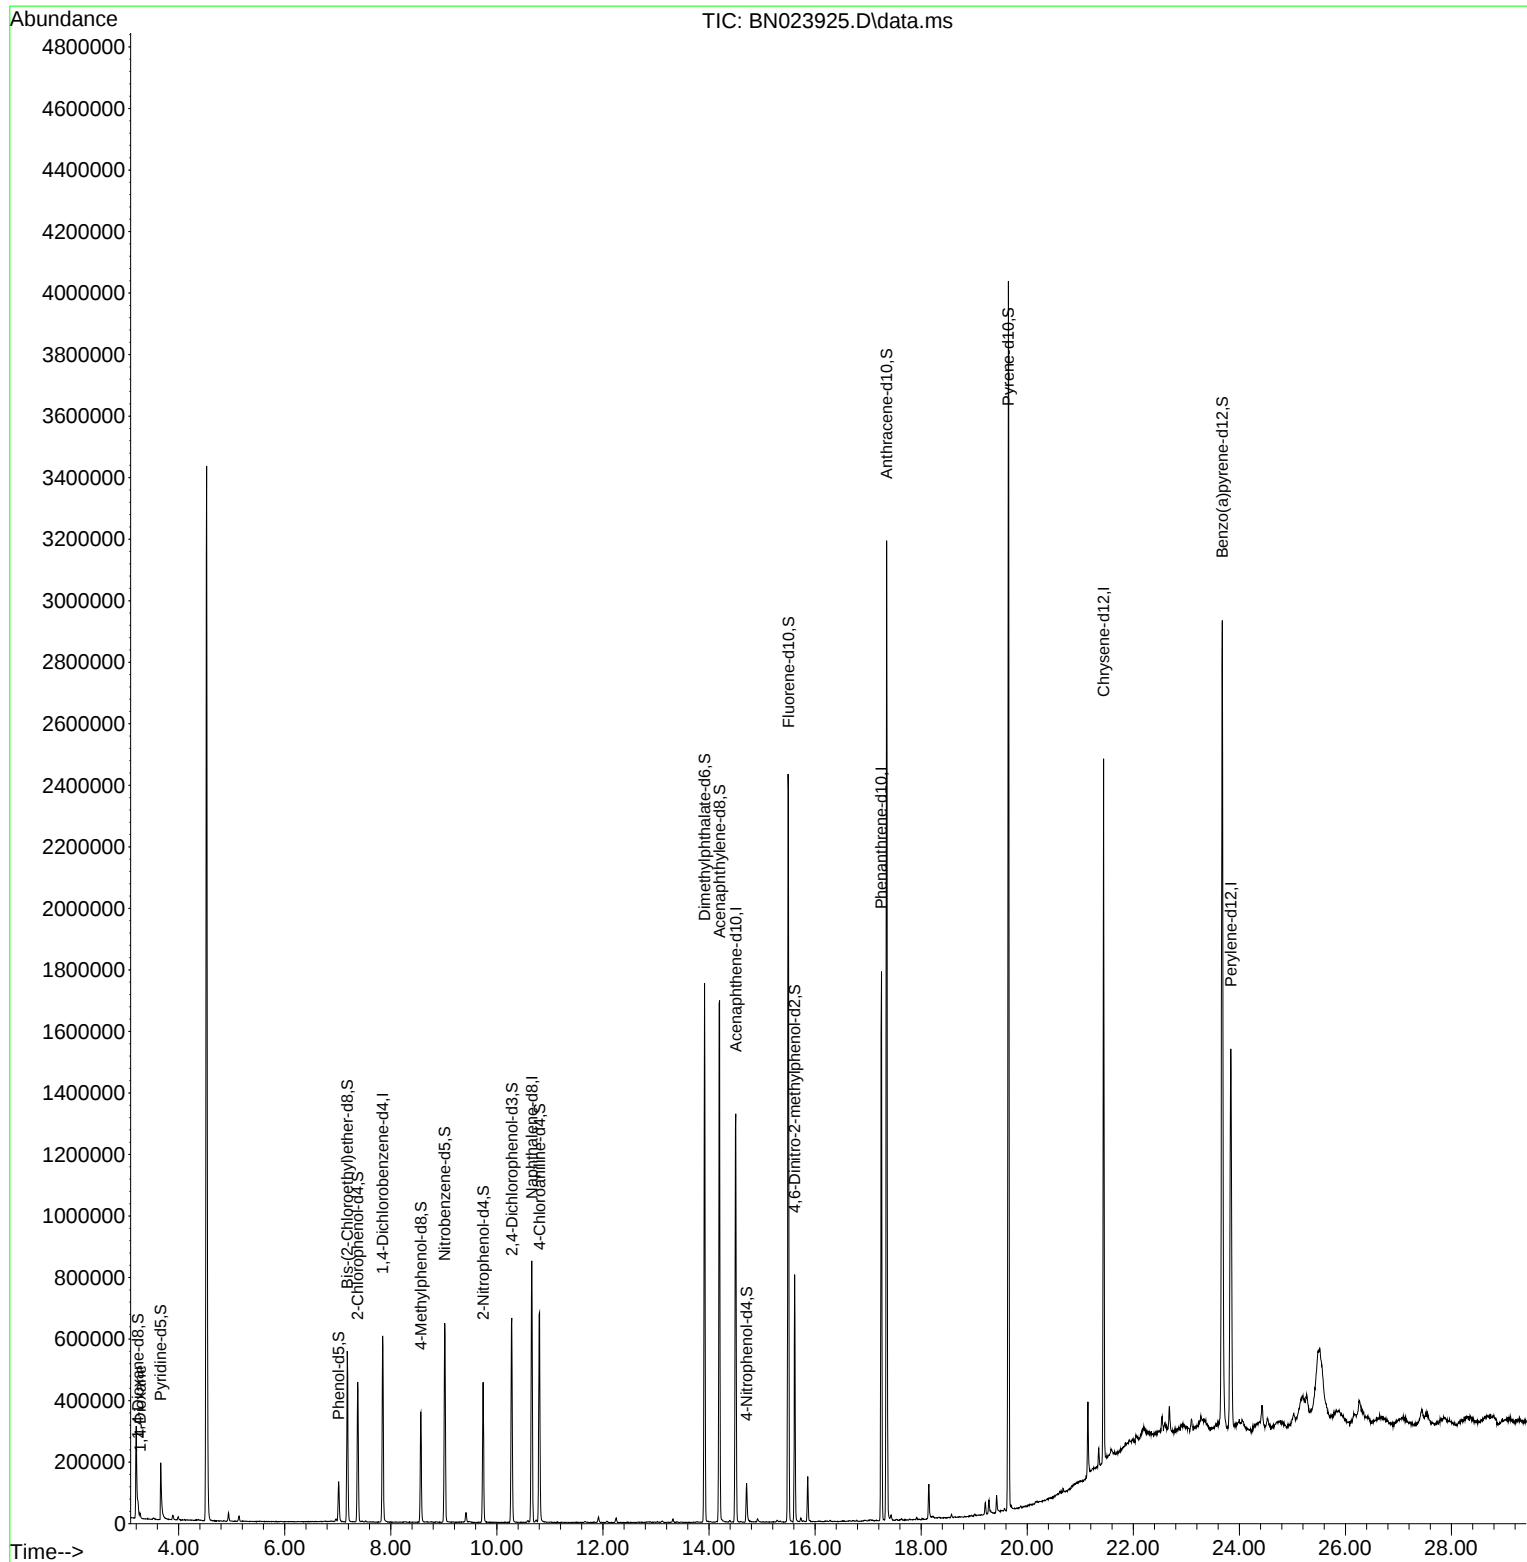

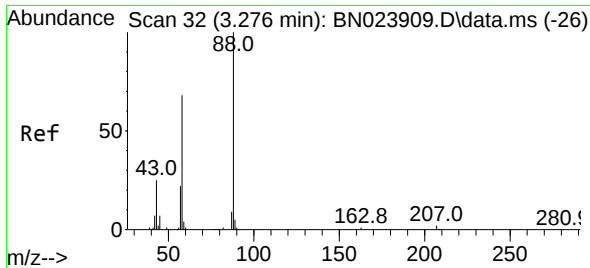

#2
 1,4-Dioxane
 Concen: 2.175 ng/uL
 RT: 3.275 min Scan# 31
 Delta R.T. -0.001 min
 Lab File: BN023925.D
 Acq: 03 Feb 2023 03:33

Instrument :
 BNA_N
 ClientSampleId :
 C0LC6

Tgt Ion: 88 Resp: 8473
 Ion Ratio Lower Upper
 88 100
 43 30.7 42.1 63.1#
 58 60.4 53.8 80.6

