

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023897.D
 Acq On : 02 Feb 2023 09:55
 Operator : CG/JU
 Sample : PB150578BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK578

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	36	rVB	48460	74041	1.18%	0.122%
2	3.670	95	99	124	rBV	589187	1043258	16.68%	1.723%
3	3.993	150	154	163	rVB	20633	32404	0.52%	0.054%
4	7.022	660	669	679	rBV	887673	1396779	22.33%	2.306%
5	7.187	690	697	707	rBV	740685	1129399	18.06%	1.865%
6	7.381	723	730	742	rBV	929090	1452626	23.23%	2.399%
7	7.852	803	810	822	rVB	775379	1214505	19.42%	2.005%
8	8.569	925	932	943	rBV	1073586	1735336	27.75%	2.865%
9	9.022	1001	1009	1021	rBV	898389	1433895	22.93%	2.368%
10	9.746	1124	1132	1142	rBV	808071	1280590	20.47%	2.115%
11	10.281	1216	1223	1232	rBV	1165455	1874419	29.97%	3.095%
12	10.663	1280	1288	1296	rBV	1075412	1764927	28.22%	2.914%
13	10.805	1304	1312	1328	rBV	1172492	1932642	30.90%	3.191%
14	12.251	1553	1558	1563	rBV2	19952	30692	0.49%	0.051%
15	13.463	1760	1764	1772	rBV7	3139	7371	0.12%	0.012%
16	13.922	1835	1842	1849	rBV	2257155	3014363	48.20%	4.977%
17	14.198	1882	1889	1898	rBV2	2390731	3405191	54.44%	5.623%
18	14.504	1934	1941	1952	rBV	1785799	2505900	40.07%	4.138%
19	14.716	1971	1977	1994	rBV	1174551	1631972	26.09%	2.695%
20	15.287	2069	2074	2081	rBV7	5310	10468	0.17%	0.017%
21	15.498	2103	2110	2123	rVB	3072420	4273783	68.33%	7.057%
22	15.622	2124	2131	2143	rVV	1191503	1614219	25.81%	2.665%
23	15.734	2146	2150	2154	rVB3	13451	18711	0.30%	0.031%
24	17.251	2402	2408	2416	rBV	2269828	3204765	51.24%	5.292%
25	17.351	2419	2425	2440	rVV2	3526783	4786997	76.54%	7.904%
26	19.210	2736	2741	2747	rBV	47552	63313	1.01%	0.105%
27	19.281	2749	2753	2759	rVB	41114	56583	0.90%	0.093%
28	19.428	2776	2778	2781	rBV4	6432	6926	0.11%	0.011%
29	19.651	2809	2816	2822	rBV	4341573	5837330	93.33%	9.639%
30	21.445	3116	3121	3127	rBV	2932303	3728188	59.61%	6.156%
31	23.692	3495	3503	3518	rVB2	3009081	6254479	100.00%	10.327%
32	23.851	3523	3530	3540	rVV2	1986291	3745573	59.89%	6.185%




Sum of corrected areas: 60561645

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023897.D
Acq On : 02 Feb 2023 09:55
Operator : CG/JU
Sample : PB150578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK578

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

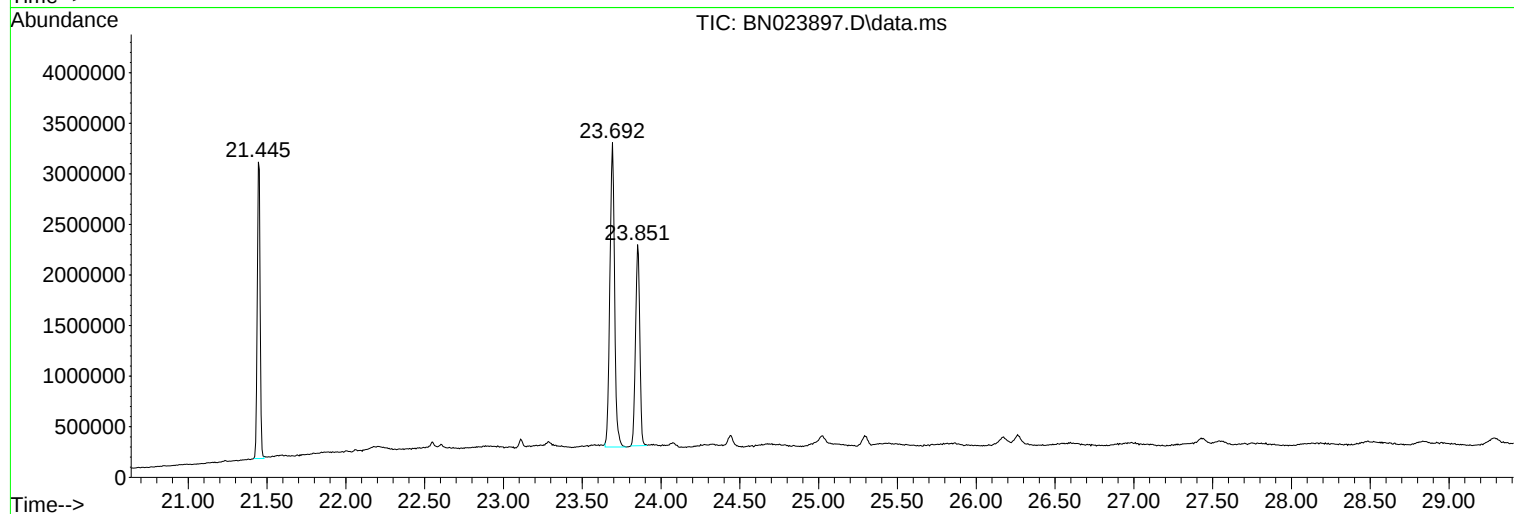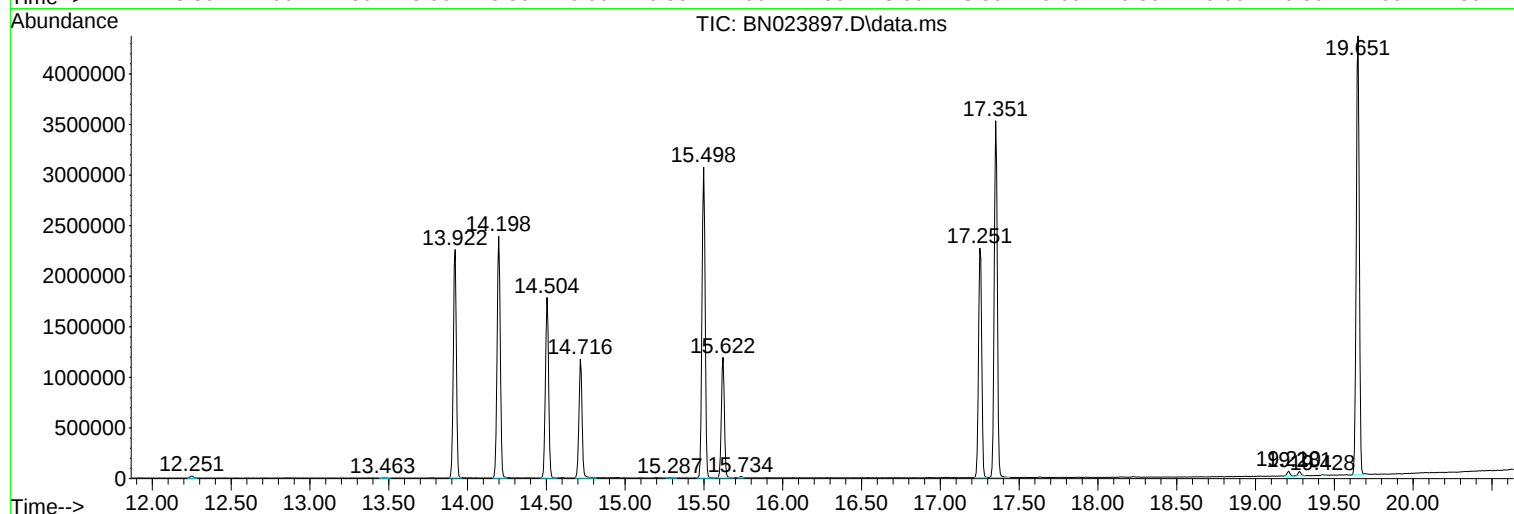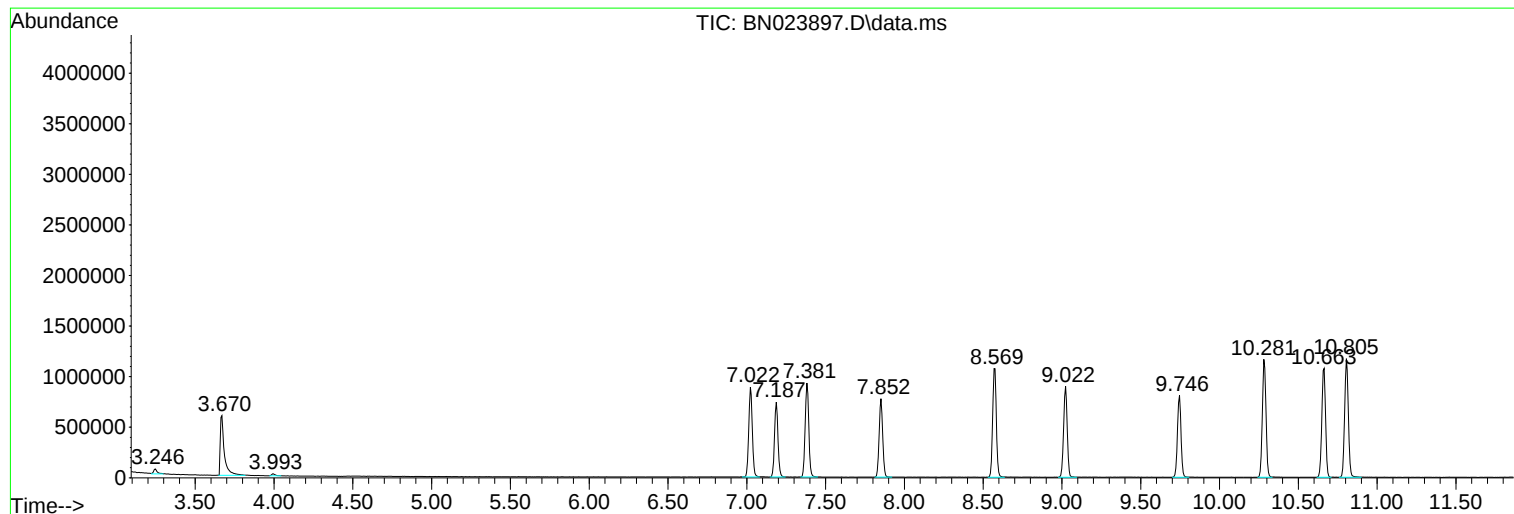

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023897.D
Acq On : 02 Feb 2023 09:55
Operator : CG/JU
Sample : PB150578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK578

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023897.D
Acq On : 02 Feb 2023 09:55
Operator : CG/JU
Sample : PB150578BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK578

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc