

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023910.D
 Acq On : 02 Feb 2023 18:21
 Operator : CG/JU
 Sample : PB150495BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	34	rVB	42034	55390	1.36%	0.131%
2	3.663	94	98	114	rBV	499341	750420	18.42%	1.773%
3	3.993	150	154	159	rVB	10518	14315	0.35%	0.034%
4	7.022	663	669	679	rVB	665105	984724	24.17%	2.326%
5	7.187	690	697	708	rVB	527143	795820	19.53%	1.880%
6	7.381	723	730	741	rVB	685573	1037363	25.46%	2.451%
7	7.851	803	810	818	rBV	588023	885485	21.73%	2.092%
8	8.569	923	932	942	rBV	811480	1243809	30.53%	2.938%
9	9.022	1001	1009	1018	rBV	640608	997997	24.49%	2.358%
10	9.745	1125	1132	1143	rBV	556423	884180	21.70%	2.089%
11	10.281	1217	1223	1236	rBV	829477	1346694	33.05%	3.182%
12	10.663	1280	1288	1296	rBV	788803	1302486	31.97%	3.077%
13	10.804	1305	1312	1323	rBV	839306	1372133	33.67%	3.242%
14	12.251	1553	1558	1565	rBV2	14080	22179	0.54%	0.052%
15	12.857	1656	1661	1667	rBV8	2545	4755	0.12%	0.011%
16	13.775	1814	1817	1821	rBV5	3441	4700	0.12%	0.011%
17	13.922	1833	1842	1853	rBV	1682264	2245148	55.10%	5.304%
18	14.198	1882	1889	1903	rBV	1761692	2453166	60.21%	5.796%
19	14.504	1932	1941	1948	rBV	1338621	1899794	46.62%	4.488%
20	14.716	1971	1977	1990	rBV	772758	1070890	26.28%	2.530%
21	15.286	2070	2074	2078	rVB5	3446	4643	0.11%	0.011%
22	15.498	2103	2110	2118	rBV	2303180	3164656	77.67%	7.476%
23	15.622	2125	2131	2145	rBV	782534	1013359	24.87%	2.394%
24	15.733	2145	2150	2155	rVV3	9473	13239	0.32%	0.031%
25	15.786	2155	2159	2164	rBV3	7145	10079	0.25%	0.024%
26	16.092	2207	2211	2220	rVB7	4790	10312	0.25%	0.024%
27	17.033	2370	2371	2377	rVB3	3694	4408	0.11%	0.010%
28	17.251	2402	2408	2419	rBV	1684802	2368315	58.12%	5.595%
29	17.351	2419	2425	2436	rBV	2569879	3583855	87.96%	8.467%
30	17.633	2470	2473	2479	rVB4	4885	6753	0.17%	0.016%
31	17.863	2510	2512	2517	rVB6	4610	5437	0.13%	0.013%
32	18.227	2570	2574	2576	rBV4	3897	5648	0.14%	0.013%
33	19.210	2737	2741	2747	rVB3	29870	40554	1.00%	0.096%
34	19.280	2749	2753	2758	rBV	32137	41944	1.03%	0.099%
35	19.651	2810	2816	2821	rBV	3239123	4074642	100.00%	9.626%
36	21.362	3103	3107	3114	rBV	230361	283896	6.97%	0.671%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023910.D
Acq On : 02 Feb 2023 18:21
Operator : CG/JU
Sample : PB150495BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Title : SVOA CALIBRATION

37	21.451	3117	3122	3130	rVV	1952735	2414621	59.26%	5.705%
38	23.692	3496	3503	3515	rVB2	1829288	3701943	90.85%	8.746%
39	23.851	3524	3530	3542	rBV2	1174651	2208316	54.20%	5.217%




Sum of corrected areas: 42328068

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023910.D
Acq On : 02 Feb 2023 18:21
Operator : CG/JU
Sample : PB150495BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

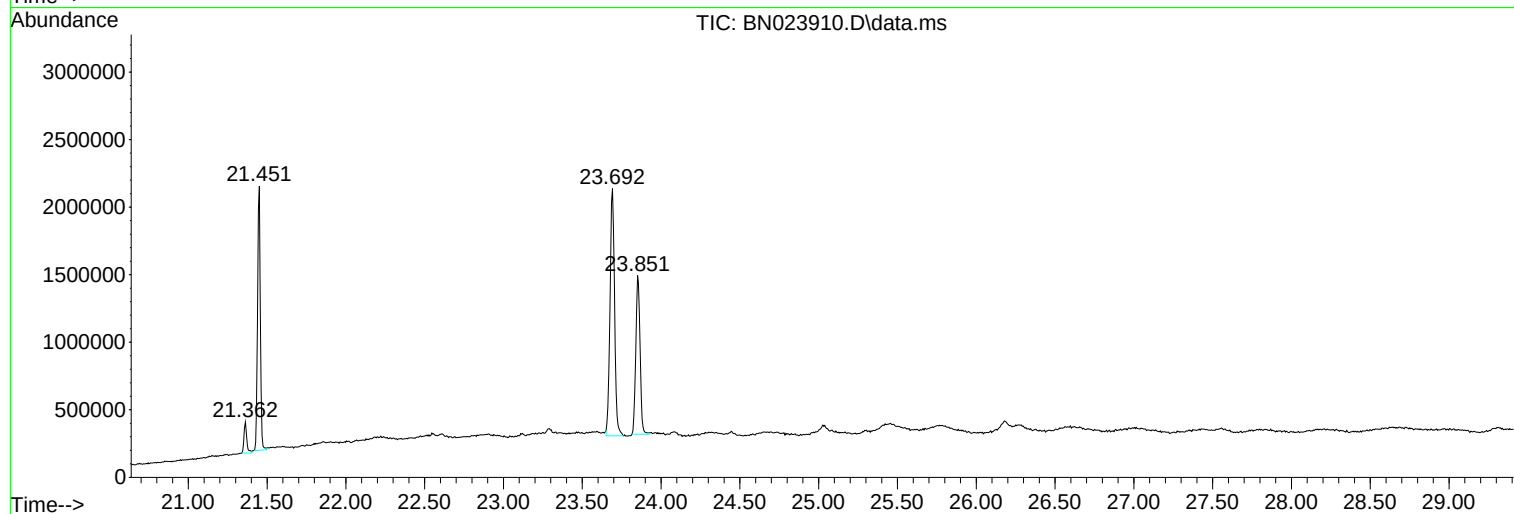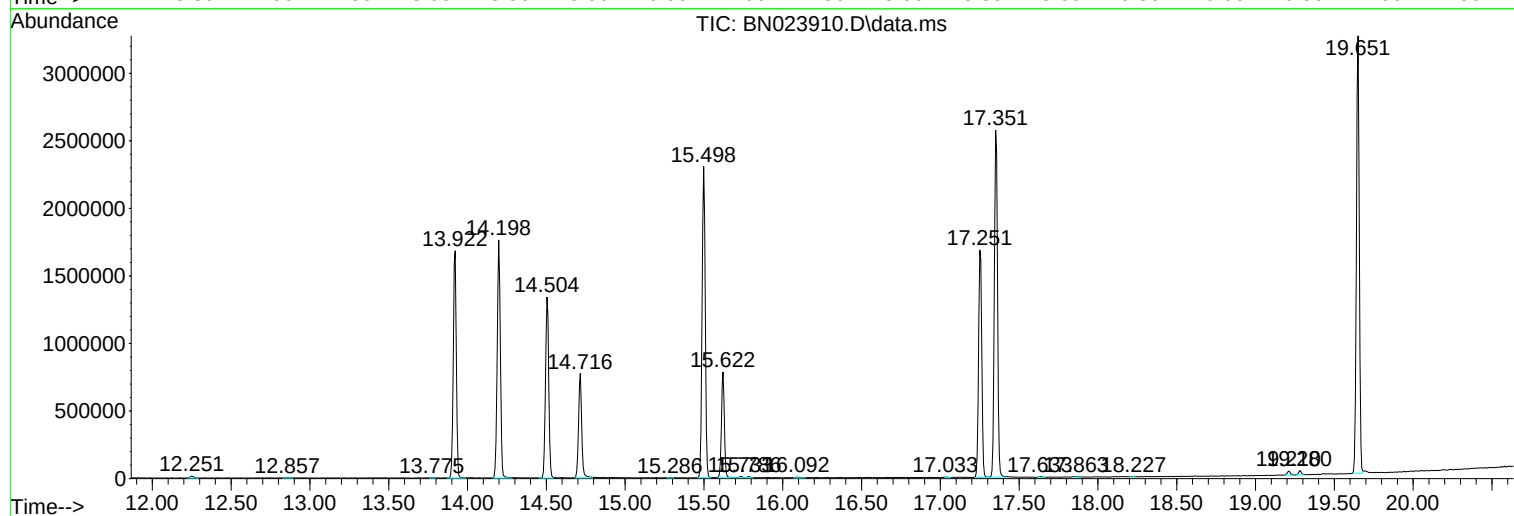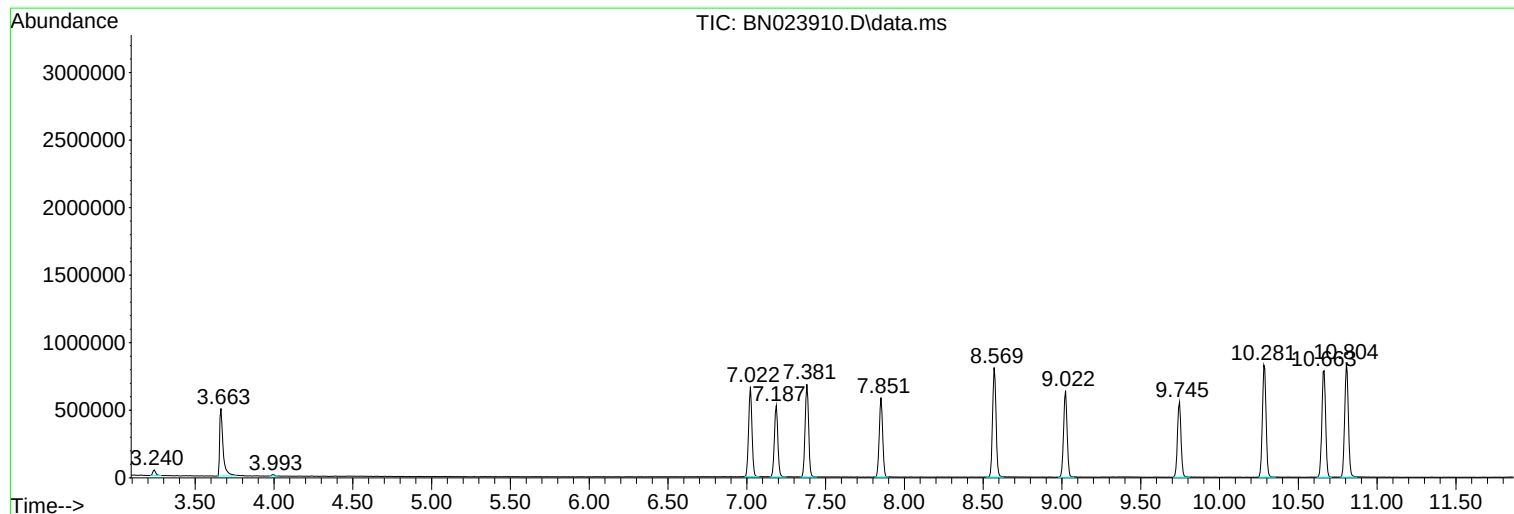

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023910.D
Acq On : 02 Feb 2023 18:21
Operator : CG/JU
Sample : PB150495BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phthalic acid, 2-ethylhexyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.363	2.35 ng/ul	283896	Chrysene-d12	21.451

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	90
2			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	87
3			Phthalic acid, 2-ethylhexyl isoh...	362	C22H34O4	1000308-98-5	78
4			Phthalic acid, di(oct-3-yl) ester	390	C24H38O4	1000377-72-3	78
5			Bis(2-ethylhexyl) phthalate	390	C24H38O4	000117-81-7	68

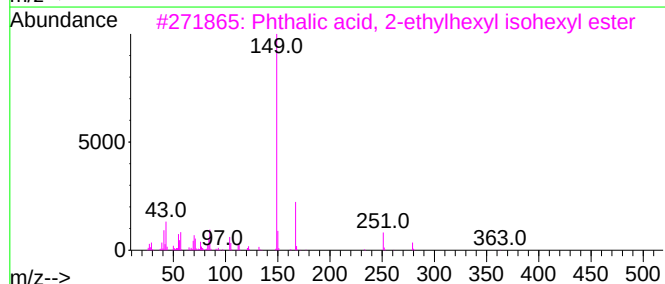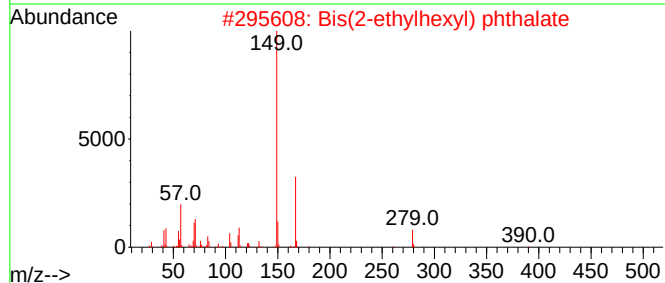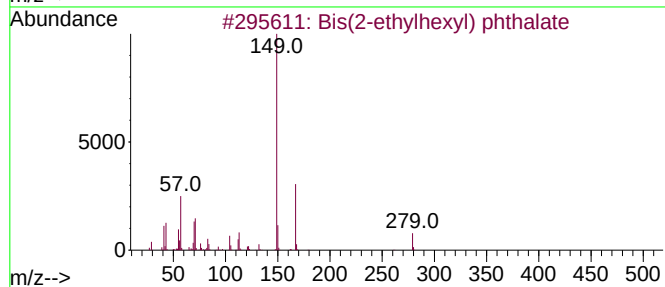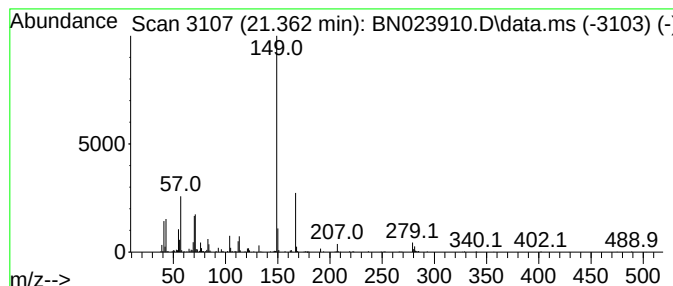

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023910.D
Acq On : 02 Feb 2023 18:21
Operator : CG/JU
Sample : PB150495BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phthalic acid, ...	21.363	2.4	ng/ul	283896	5	21.451	2414620	20.0