

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023911.D
 Acq On : 02 Feb 2023 18:58
 Operator : CG/JU
 Sample : PB150496BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK496

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	36	rVB	45970	62502	1.40%	0.142%
2	3.664	95	98	116	rBV	559478	840531	18.79%	1.905%
3	3.993	150	154	160	rVB	10660	14512	0.32%	0.033%
4	7.022	662	669	683	rVB	725291	1092806	24.43%	2.477%
5	7.187	691	697	709	rVB	589871	875852	19.58%	1.985%
6	7.381	724	730	744	rVB	754343	1135491	25.39%	2.574%
7	7.852	804	810	817	rBV	538984	805406	18.01%	1.826%
8	8.569	925	932	942	rBV	908133	1378762	30.82%	3.126%
9	9.022	1000	1009	1023	rVB	718245	1104112	24.68%	2.503%
10	9.746	1124	1132	1143	rBV	628493	983563	21.99%	2.230%
11	10.281	1215	1223	1232	rBV	932661	1490349	33.32%	3.378%
12	10.663	1281	1288	1299	rVB	704622	1186893	26.54%	2.691%
13	10.805	1305	1312	1325	rBV	943091	1518063	33.94%	3.441%
14	12.252	1553	1558	1563	rBV	16112	25063	0.56%	0.057%
15	13.922	1835	1842	1850	rBV	1785606	2444078	54.64%	5.540%
16	14.199	1882	1889	1904	rBV	1886618	2705056	60.48%	6.132%
17	14.504	1935	1941	1949	rVB	1216180	1727146	38.61%	3.915%
18	14.716	1969	1977	1996	rBV	858367	1202160	26.88%	2.725%
19	15.287	2069	2074	2078	rBV6	4649	7513	0.17%	0.017%
20	15.498	2102	2110	2118	rBV	2493683	3478486	77.77%	7.885%
21	15.622	2124	2131	2142	rBV	908742	1162102	25.98%	2.634%
22	15.734	2145	2150	2155	rVV	10475	13676	0.31%	0.031%
23	15.781	2155	2158	2164	rVB6	6650	8014	0.18%	0.018%
24	16.093	2208	2211	2218	rVB6	4418	6444	0.14%	0.015%
25	17.251	2401	2408	2418	rBV	1559933	2141144	47.87%	4.854%
26	17.351	2418	2425	2441	rVV2	2857014	3907114	87.35%	8.857%
27	17.634	2470	2473	2478	rVB4	4137	6357	0.14%	0.014%
28	17.851	2506	2510	2513	rBV5	4777	7188	0.16%	0.016%
29	18.228	2570	2574	2579	rBV4	3982	6189	0.14%	0.014%
30	19.210	2737	2741	2745	rVB2	34679	46313	1.04%	0.105%
31	19.281	2749	2753	2759	rVB	30902	42803	0.96%	0.097%
32	19.528	2793	2795	2798	rBV3	5127	5512	0.12%	0.012%
33	19.651	2809	2816	2822	rBV	3328837	4472878	100.00%	10.140%
34	21.357	3102	3106	3110	rBV	206190	239320	5.35%	0.543%
35	21.445	3116	3121	3127	rBV	1750369	2154460	48.17%	4.884%
36	23.698	3496	3504	3516	rBV2	1957249	3881788	86.79%	8.800%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023911.D
Acq On : 02 Feb 2023 18:58
Operator : CG/JU
Sample : PB150496BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK496

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Title : SVOA CALIBRATION

37	23.839	3522	3528	3536	rVB2	1034816	1933392	43.22%	4.383%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 44113038

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023911.D
Acq On : 02 Feb 2023 18:58
Operator : CG/JU
Sample : PB150496BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

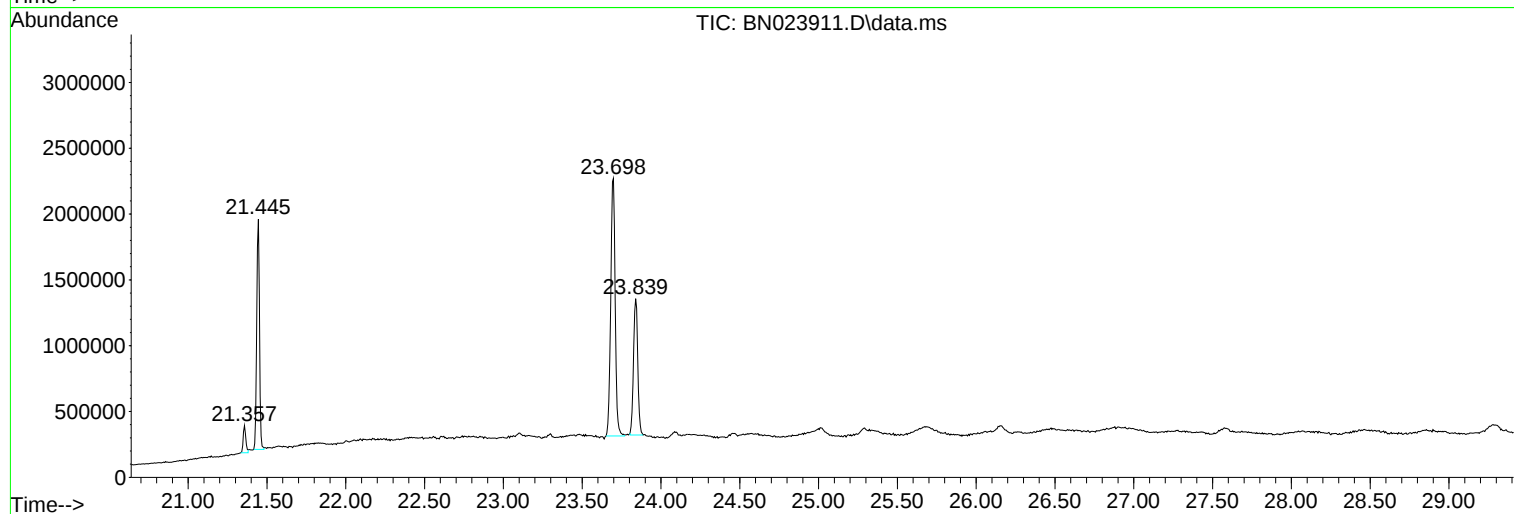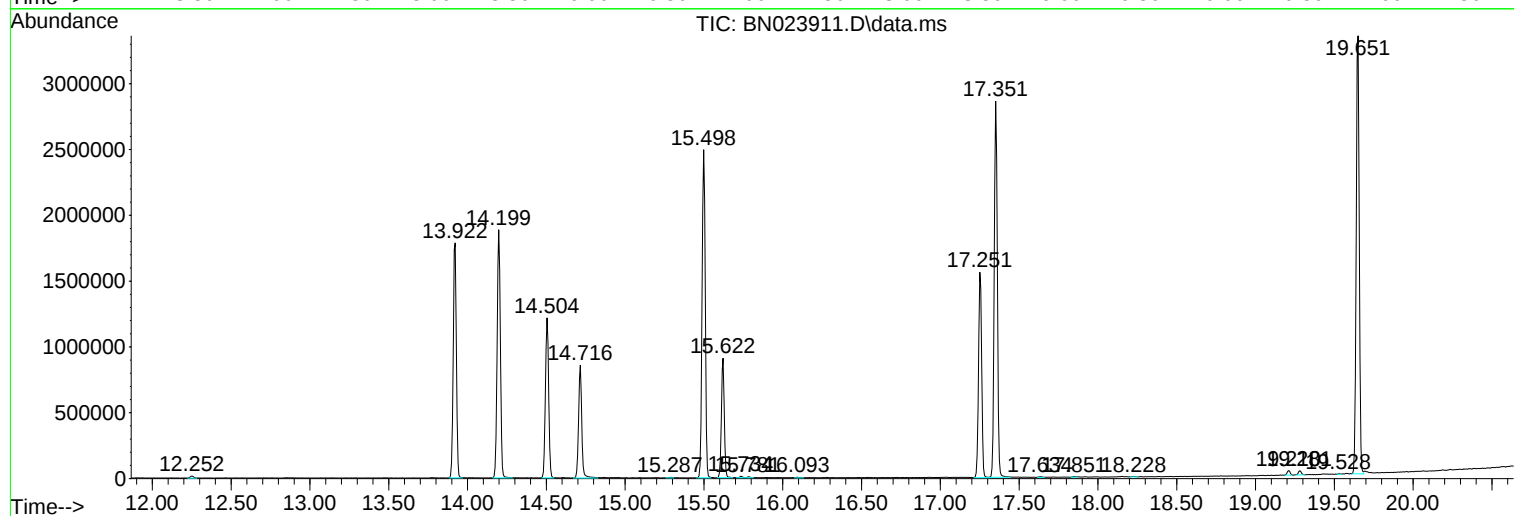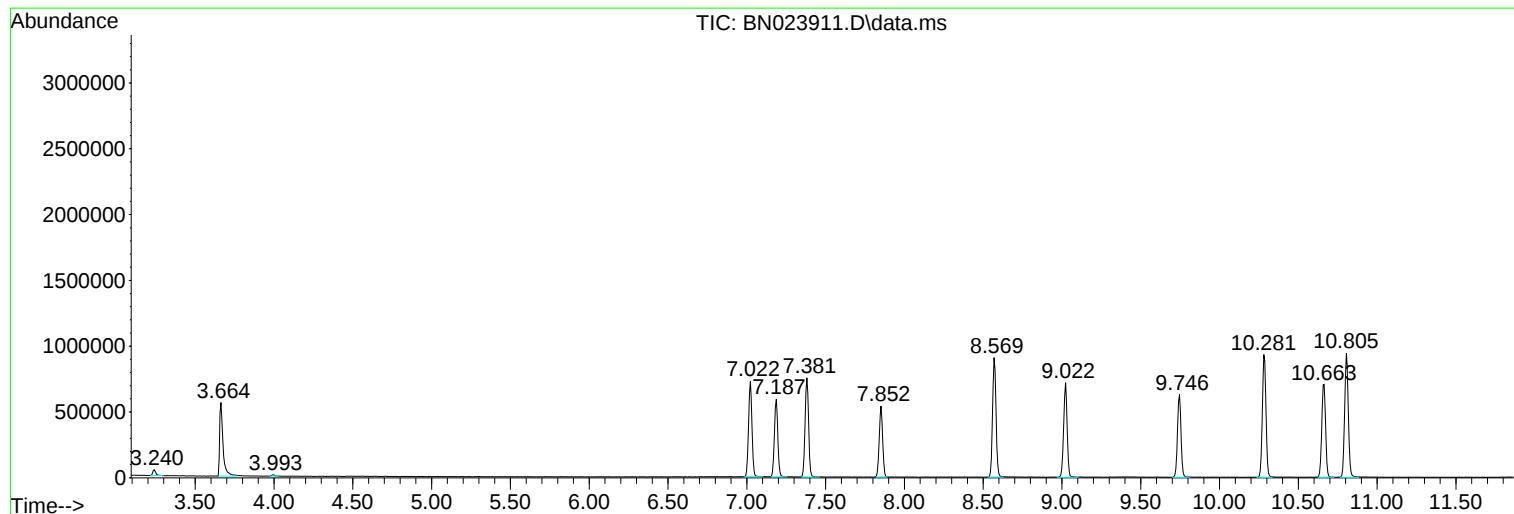

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023911.D
Acq On : 02 Feb 2023 18:58
Operator : CG/JU
Sample : PB150496BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023911.D
Acq On : 02 Feb 2023 18:58
Operator : CG/JU
Sample : PB150496BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc