

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023914.D
 Acq On : 02 Feb 2023 20:49
 Operator : CG/JU
 Sample : 01294-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	36	rVB	37757	52656	1.01%	0.111%
2	3.528	72	75	85	rVB4	7241	14458	0.28%	0.031%
3	3.664	95	98	114	rBV	190967	305946	5.84%	0.646%
4	3.899	132	138	144	rVB	18194	30474	0.58%	0.064%
5	3.993	150	154	160	rVB2	12628	18461	0.35%	0.039%
6	4.134	173	178	181	rVB4	4004	5989	0.11%	0.013%
7	5.140	342	349	355	rVB	38082	57424	1.10%	0.121%
8	5.387	387	391	394	rBV2	5033	7221	0.14%	0.015%
9	6.969	655	660	663	rBV4	6199	9328	0.18%	0.020%
10	7.022	663	669	677	rVB	149284	230422	4.40%	0.487%
11	7.187	690	697	709	rBV	606364	934529	17.84%	1.974%
12	7.381	723	730	737	rBV	626290	943327	18.01%	1.993%
13	7.787	795	799	803	rBV5	7073	10413	0.20%	0.022%
14	7.852	803	810	820	rVV	586694	914529	17.46%	1.932%
15	8.204	864	870	875	rBV	20643	31611	0.60%	0.067%
16	8.569	926	932	941	rBV	474662	726651	13.87%	1.535%
17	9.022	1001	1009	1012	rBV	738456	1180108	22.53%	2.493%
18	9.063	1012	1016	1024	rVB	1078568	1683184	32.13%	3.556%
19	9.422	1070	1077	1083	rBV2	21699	32371	0.62%	0.068%
20	9.575	1098	1103	1107	rBV5	3927	7617	0.15%	0.016%
21	9.740	1124	1131	1146	rBV	611470	998160	19.05%	2.109%
22	10.040	1177	1182	1190	rVB2	12385	20574	0.39%	0.043%
23	10.281	1216	1223	1239	rBV	939725	1493478	28.51%	3.155%
24	10.657	1280	1287	1297	rVB	833718	1321953	25.24%	2.793%
25	10.804	1304	1312	1321	rBV	550640	905209	17.28%	1.912%
26	11.793	1473	1480	1486	rBV	35408	60096	1.15%	0.127%
27	11.922	1496	1502	1505	rBV2	11231	16808	0.32%	0.036%
28	11.998	1508	1515	1524	rBV2	10073	18411	0.35%	0.039%
29	12.075	1524	1528	1534	rVB4	3652	6661	0.13%	0.014%
30	12.245	1552	1557	1564	rVB	16205	26129	0.50%	0.055%
31	12.540	1601	1607	1611	rBV2	11640	18611	0.36%	0.039%
32	13.322	1736	1740	1745	rVB2	9312	11812	0.23%	0.025%
33	13.916	1835	1841	1851	rBV	2028185	2806568	53.58%	5.929%
34	14.198	1882	1889	1901	rVV	2113150	3004434	57.35%	6.347%
35	14.392	1917	1922	1926	rVB5	5601	7926	0.15%	0.017%
36	14.504	1934	1941	1946	rBV	1355957	1884412	35.97%	3.981%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023914.D
 Acq On : 02 Feb 2023 20:49
 Operator : CG/JU
 Sample : 01294-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

37	14.545	1946	1948	1954	rVV2	27970	45666	0.87%	0.096%
38	14.710	1970	1976	1985	rBV	157830	237782	4.54%	0.502%
39	14.869	1999	2003	2007	rBV4	6291	8897	0.17%	0.019%
40	14.922	2007	2012	2019	rVB7	13304	23827	0.45%	0.050%
41	15.286	2070	2074	2078	rVV5	6160	8565	0.16%	0.018%
42	15.498	2103	2110	2116	rVV	2897418	3955194	75.50%	8.356%
43	15.545	2116	2118	2123	rVB3	22804	23611	0.45%	0.050%
44	15.622	2124	2131	2139	rBV	1089911	1440179	27.49%	3.042%
45	15.733	2146	2150	2155	rBV	13346	18419	0.35%	0.039%
46	15.781	2155	2158	2163	rVB5	6714	9105	0.17%	0.019%
47	15.863	2168	2172	2177	rVB	76681	98764	1.89%	0.209%
48	16.281	2239	2243	2248	rBV7	3588	5683	0.11%	0.012%
49	16.651	2302	2306	2309	rBV6	7156	8140	0.16%	0.017%
50	17.010	2364	2367	2370	rVV5	5407	8308	0.16%	0.018%
51	17.039	2370	2372	2376	rVB5	5090	6164	0.12%	0.013%
52	17.128	2383	2387	2390	rBV3	12708	16476	0.31%	0.035%
53	17.251	2402	2408	2416	rBV	1707660	2323228	44.35%	4.908%
54	17.351	2418	2425	2433	rVV	3197484	4417577	84.33%	9.332%
55	17.433	2436	2439	2448	rVB9	15537	25743	0.49%	0.054%
56	17.633	2470	2473	2477	rVB6	6556	7563	0.14%	0.016%
57	17.792	2496	2500	2504	rBV6	3583	5503	0.11%	0.012%
58	17.922	2520	2522	2525	rVB4	7922	8266	0.16%	0.017%
59	18.145	2555	2560	2568	rBV	162352	227013	4.33%	0.480%
60	18.575	2629	2633	2637	rBV7	13687	18148	0.35%	0.038%
61	18.633	2638	2643	2648	rVB8	13355	24866	0.47%	0.053%
62	19.004	2703	2706	2714	rVB7	12853	19695	0.38%	0.042%
63	19.210	2737	2741	2746	rBV2	46762	67038	1.28%	0.142%
64	19.280	2749	2753	2764	rVB	51267	91011	1.74%	0.192%
65	19.427	2774	2778	2782	rBV2	81893	113465	2.17%	0.240%
66	19.651	2809	2816	2821	rBV	3885953	5238512	100.00%	11.067%
67	21.151	3067	3071	3078	rBV2	196797	265485	5.07%	0.561%
68	21.357	3103	3106	3110	rBV	187973	190932	3.64%	0.403%
69	21.445	3116	3121	3126	rBV	1825883	2302655	43.96%	4.864%
70	23.686	3495	3502	3517	rVB	2145096	4314604	82.36%	9.115%
71	23.851	3524	3530	3539	rVB2	1024248	1962005	37.45%	4.145%




Sum of corrected areas: 47336050

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023914.D
Acq On : 02 Feb 2023 20:49
Operator : CG/JU
Sample : 01294-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

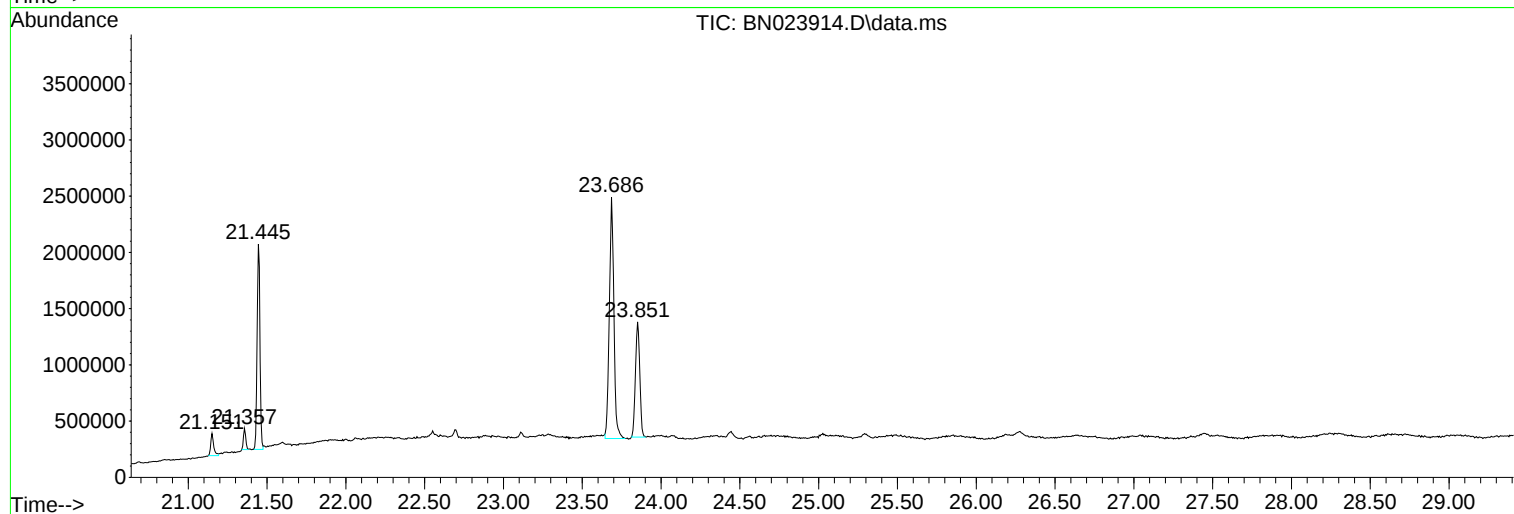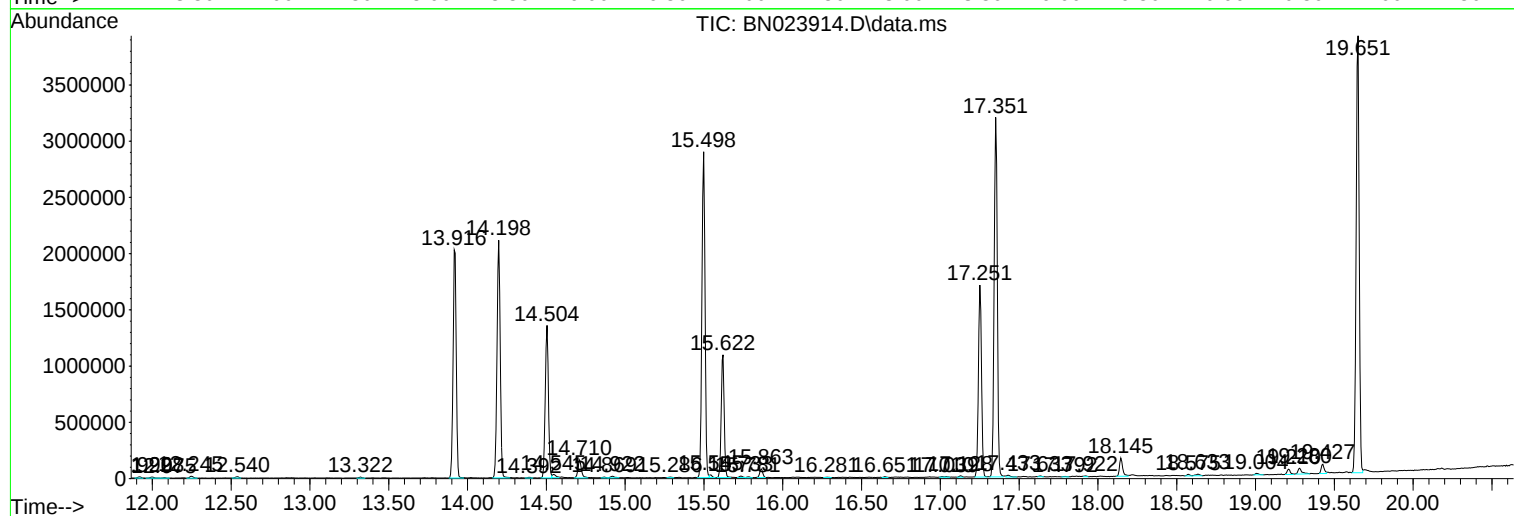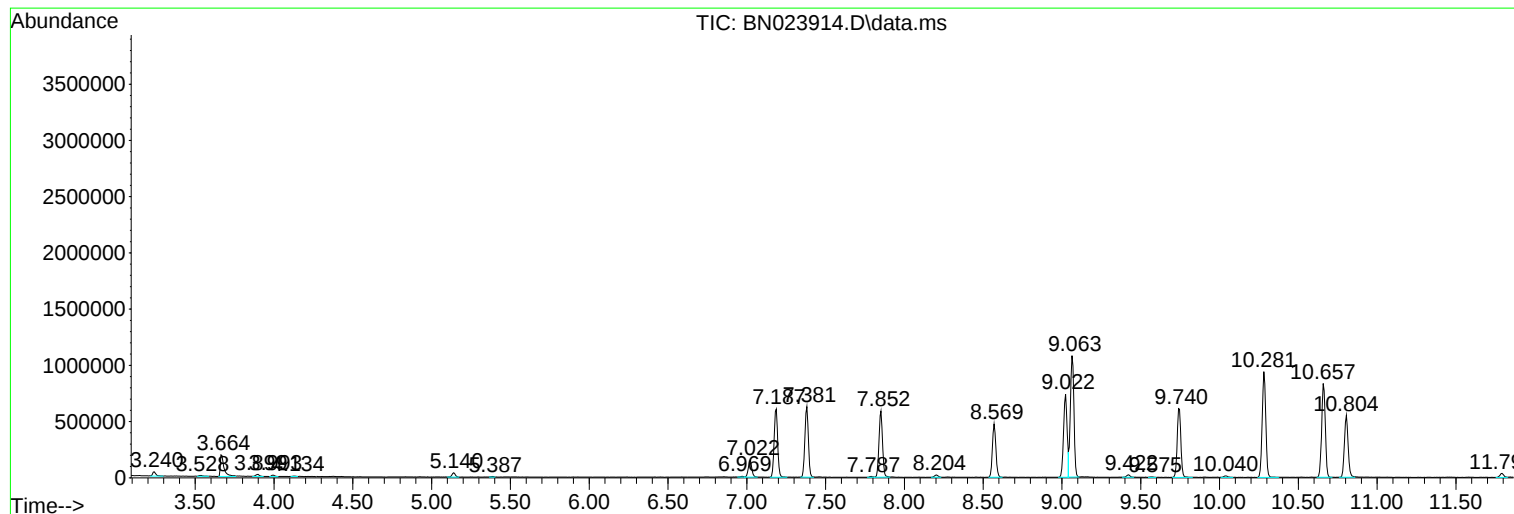

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023914.D
Acq On : 02 Feb 2023 20:49
Operator : CG/JU
Sample : 01294-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.151 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.151	2.31 ng/ul	265485	Chrysene-d12	21.445

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetradecane	196	C14H28	000295-17-0	98
2			E-14-Hexadecenal	238	C16H30O	330207-53-9	95
3			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
5			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94

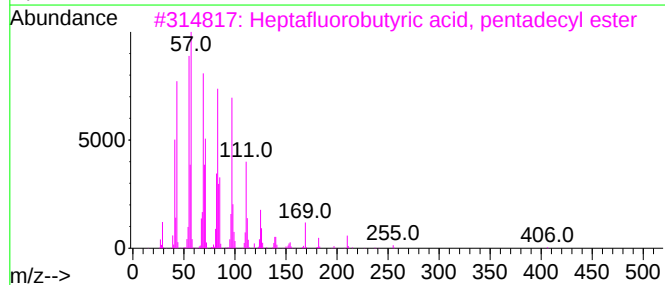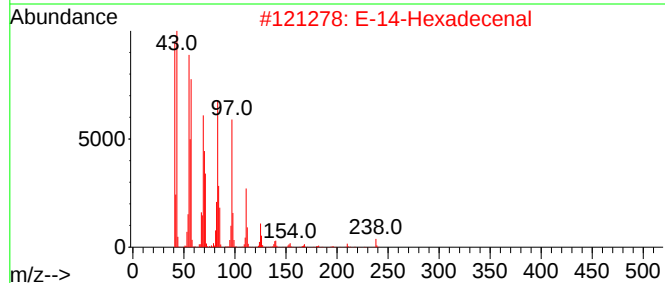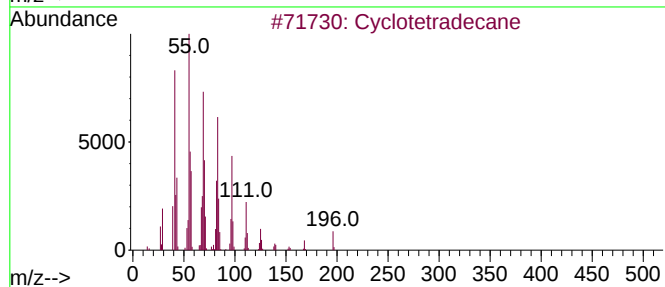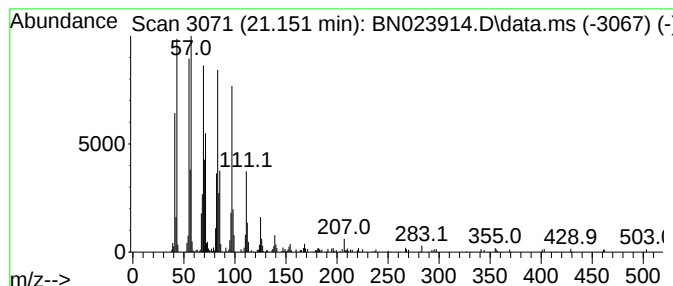

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023914.D
Acq On : 02 Feb 2023 20:49
Operator : CG/JU
Sample : 01294-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.151	2.3	ng/u1	265485	5	21.445	2302660	20.0