

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023917.D
 Acq On : 02 Feb 2023 22:40
 Operator : CG/JU
 Sample : 01294-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	36	rVB	35706	51731	0.95%	0.109%
2	3.663	95	98	111	rBV	161793	258268	4.72%	0.545%
3	3.899	133	138	145	rVB2	16742	26394	0.48%	0.056%
4	3.993	150	154	161	rVB	14665	19217	0.35%	0.041%
5	4.946	311	316	319	rVB4	6609	9052	0.17%	0.019%
6	7.022	663	669	676	rVB	177956	269568	4.93%	0.569%
7	7.181	690	696	706	rBV	589998	926626	16.94%	1.957%
8	7.381	723	730	740	rBV	607207	941383	17.21%	1.988%
9	7.851	801	810	818	rBV	609738	938563	17.16%	1.982%
10	8.569	924	932	942	rBV	503779	780728	14.27%	1.649%
11	9.022	1002	1009	1018	rBV	739082	1180087	21.57%	2.492%
12	9.416	1073	1076	1082	rVB4	9534	15225	0.28%	0.032%
13	9.739	1124	1131	1140	rBV	619150	1004858	18.37%	2.122%
14	10.281	1216	1223	1231	rBV	920032	1464901	26.78%	3.094%
15	10.586	1269	1275	1279	rBV6	3889	6974	0.13%	0.015%
16	10.657	1279	1287	1295	rBV	859882	1391998	25.45%	2.940%
17	10.804	1303	1312	1326	rBV	879990	1456487	26.62%	3.076%
18	11.916	1496	1501	1507	rVB2	13608	22023	0.40%	0.047%
19	12.245	1553	1557	1565	rVB	16854	25576	0.47%	0.054%
20	13.775	1813	1817	1825	rBV6	3293	5828	0.11%	0.012%
21	13.916	1835	1841	1851	rBV	2001860	2753946	50.34%	5.816%
22	14.198	1882	1889	1901	rBV	2092230	3003529	54.90%	6.343%
23	14.504	1934	1941	1947	rBV	1420312	2004059	36.63%	4.232%
24	14.710	1970	1976	1993	rBV	181378	278026	5.08%	0.587%
25	14.927	2007	2013	2016	rBV7	5963	11846	0.22%	0.025%
26	15.498	2100	2110	2124	rBV	2928618	4069128	74.38%	8.593%
27	15.621	2124	2131	2145	rBV	1053613	1401643	25.62%	2.960%
28	15.733	2145	2150	2154	rVV3	13244	20077	0.37%	0.042%
29	15.786	2155	2159	2165	rVB5	4708	6751	0.12%	0.014%
30	17.010	2363	2367	2370	rBV7	4877	7325	0.13%	0.015%
31	17.251	2402	2408	2416	rBV	1853797	2488754	45.49%	5.256%
32	17.351	2418	2425	2435	rVV2	3444732	4685510	85.65%	9.895%
33	17.451	2439	2442	2450	rVB8	6960	10330	0.19%	0.022%
34	17.633	2471	2473	2478	rVB6	5616	7360	0.13%	0.016%
35	18.145	2553	2560	2567	rBV3	38484	62673	1.15%	0.132%
36	18.227	2570	2574	2577	rVV2	4696	6555	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023917.D
 Acq On : 02 Feb 2023 22:40
 Operator : CG/JU
 Sample : 01294-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M

Title : SVOA CALIBRATION

37	19.010	2701	2707	2713	rBV4	27318	51637	0.94%	0.109%
38	19.210	2737	2741	2746	rVB2	44635	56002	1.02%	0.118%
39	19.280	2749	2753	2758	rBV	44180	61906	1.13%	0.131%
40	19.421	2774	2777	2783	rBV5	28545	38394	0.70%	0.081%
41	19.651	2809	2816	2822	rBV	4064902	5470413	100.00%	11.553%
42	21.356	3102	3106	3111	rBV2	125170	153523	2.81%	0.324%
43	21.445	3116	3121	3126	rBV	2125639	2624905	47.98%	5.543%
44	23.686	3495	3502	3517	rVB2	2377387	4906771	89.70%	10.362%
45	23.850	3523	3530	3538	rBV2	1281695	2374744	43.41%	5.015%




Sum of corrected areas: 47351294

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023917.D
Acq On : 02 Feb 2023 22:40
Operator : CG/JU
Sample : 01294-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

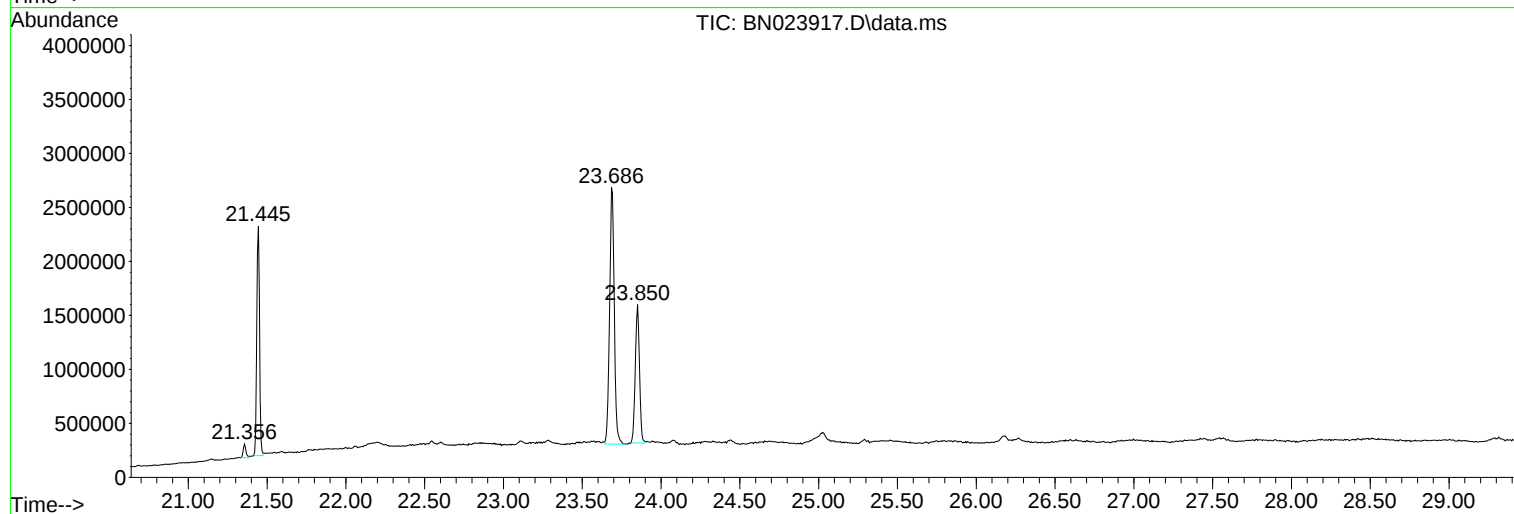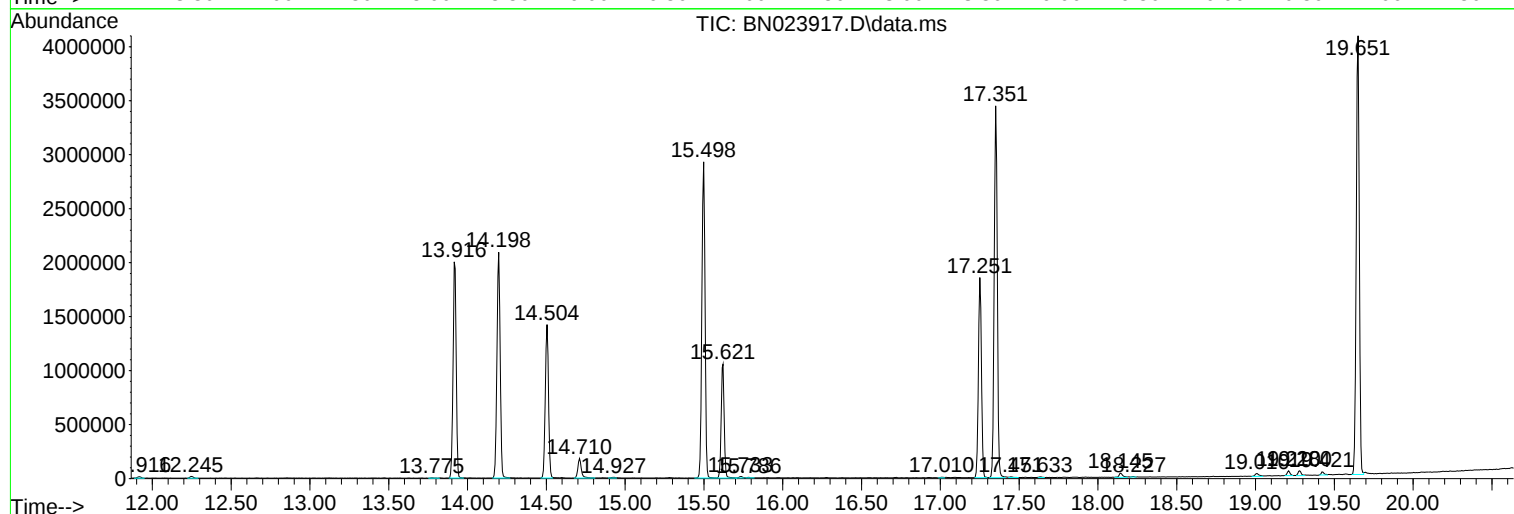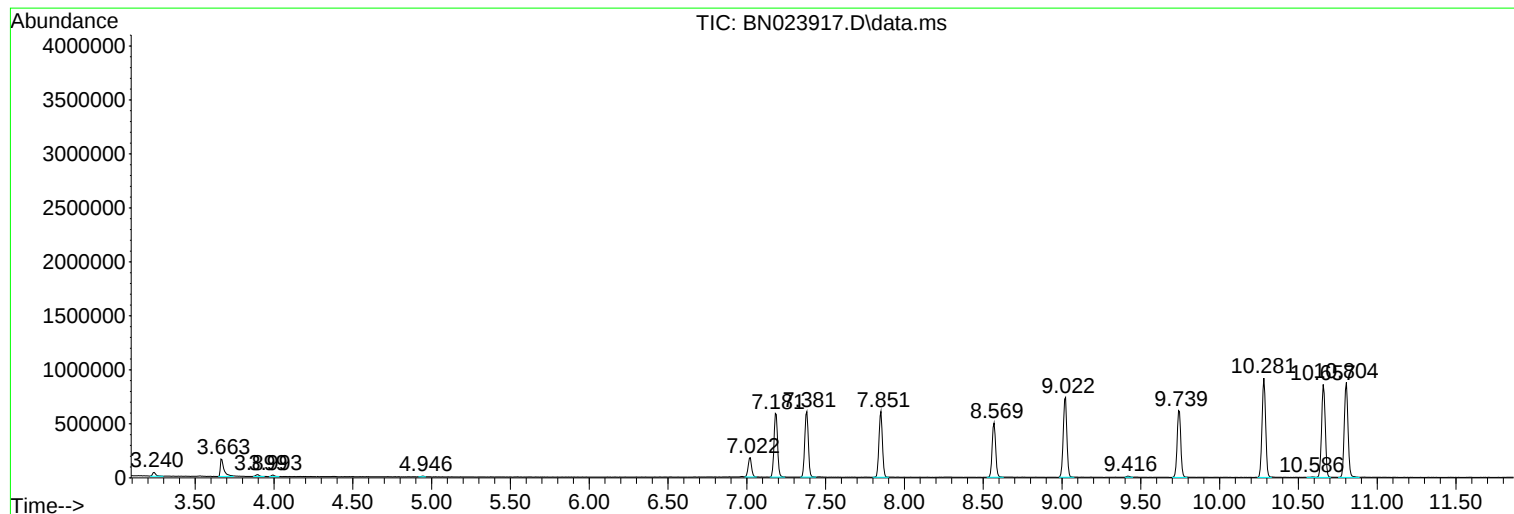

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023917.D
Acq On : 02 Feb 2023 22:40
Operator : CG/JU
Sample : 01294-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023917.D
Acq On : 02 Feb 2023 22:40
Operator : CG/JU
Sample : 01294-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc