

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023924.D
 Acq On : 03 Feb 2023 02:57
 Operator : CG/JU
 Sample : 01295-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	15	19	38	rVB2	233343	428071	8.85%	0.902%
2	3.664	96	98	115	rBV	130412	219944	4.55%	0.464%
3	3.893	133	137	144	rVB	17698	26273	0.54%	0.055%
4	3.993	148	154	161	rBV	11143	20146	0.42%	0.042%
5	4.528	238	245	260	rBV	2953083	4533289	93.77%	9.554%
6	4.946	310	316	321	rBV2	10706	17315	0.36%	0.036%
7	5.140	345	349	354	rVB5	6393	8653	0.18%	0.018%
8	7.016	663	668	677	rVB	133922	207534	4.29%	0.437%
9	7.181	690	696	706	rBV	550544	827155	17.11%	1.743%
10	7.375	721	729	740	rBV	518141	788498	16.31%	1.662%
11	7.846	801	809	817	rBV	596267	923775	19.11%	1.947%
12	7.916	817	821	828	rVB7	5318	10264	0.21%	0.022%
13	8.563	925	931	940	rBV	382900	601665	12.44%	1.268%
14	8.746	957	962	967	rBV7	3485	5508	0.11%	0.012%
15	9.016	1000	1008	1018	rBV	664316	1034238	21.39%	2.180%
16	9.422	1071	1077	1081	rBV	26704	42667	0.88%	0.090%
17	9.475	1082	1086	1091	rVB6	5419	10534	0.22%	0.022%
18	9.740	1124	1131	1141	rBV	514238	810805	16.77%	1.709%
19	10.281	1216	1223	1233	rVB	735596	1198487	24.79%	2.526%
20	10.657	1279	1287	1294	rBV	829107	1350024	27.92%	2.845%
21	10.740	1298	1301	1305	rVB4	3706	4948	0.10%	0.010%
22	10.799	1305	1311	1322	rBV	580843	988806	20.45%	2.084%
23	11.916	1494	1501	1508	rVB	31360	48944	1.01%	0.103%
24	12.075	1525	1528	1535	rVB5	5433	8329	0.17%	0.018%
25	12.245	1552	1557	1562	rBV2	13416	22510	0.47%	0.047%
26	12.857	1656	1661	1664	rBV7	3262	5416	0.11%	0.011%
27	13.110	1702	1704	1713	rVB7	4757	7113	0.15%	0.015%
28	13.322	1734	1740	1747	rVB2	13524	19858	0.41%	0.042%
29	13.916	1834	1841	1856	rBV	1705485	2250177	46.54%	4.742%
30	14.198	1882	1889	1896	rBV2	1669826	2479333	51.28%	5.225%
31	14.392	1918	1922	1928	rVB4	5815	7295	0.15%	0.015%
32	14.504	1934	1941	1947	rBV	1349639	1910478	39.52%	4.027%
33	14.710	1970	1976	1985	rBV	127762	185651	3.84%	0.391%
34	14.916	2006	2011	2016	rBV8	8149	13779	0.29%	0.029%
35	15.281	2070	2073	2079	rVV7	5211	8132	0.17%	0.017%
36	15.498	2099	2110	2123	rBV	2317235	3367823	69.66%	7.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023924.D
 Acq On : 03 Feb 2023 02:57
 Operator : CG/JU
 Sample : 01295-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

37	15.616	2123	2130	2142	rBV	812810	1053794	21.80%	2.221%
38	15.734	2146	2150	2155	rBV3	12357	16567	0.34%	0.035%
39	15.863	2167	2172	2177	rBV	136911	176111	3.64%	0.371%
40	16.716	2312	2317	2322	rVB6	3948	6986	0.14%	0.015%
41	17.251	2401	2408	2418	rBV	1793406	2390033	49.43%	5.037%
42	17.351	2418	2425	2435	rVV	3003836	4030575	83.37%	8.495%
43	17.433	2435	2439	2446	rVB3	21782	35906	0.74%	0.076%
44	17.533	2452	2456	2462	rVB6	2644	5328	0.11%	0.011%
45	17.633	2470	2473	2477	rVB6	4291	5862	0.12%	0.012%
46	17.922	2519	2522	2524	rVV4	6247	5860	0.12%	0.012%
47	18.145	2553	2560	2568	rBV	95888	142817	2.95%	0.301%
48	18.222	2570	2573	2579	rVB	8895	14050	0.29%	0.030%
49	18.575	2629	2633	2638	rBV6	13032	16854	0.35%	0.036%
50	19.210	2736	2741	2746	rBV2	39901	55642	1.15%	0.117%
51	19.280	2749	2753	2756	rBV	39957	56309	1.16%	0.119%
52	19.422	2774	2777	2785	rBV3	50656	76087	1.57%	0.160%
53	19.645	2809	2815	2821	rBV2	3642635	4834704	100.00%	10.190%
54	21.145	3066	3070	3078	rBV	245288	339027	7.01%	0.715%
55	21.357	3103	3106	3112	rBV2	70220	78266	1.62%	0.165%
56	21.445	3116	3121	3129	rVV	2182788	2664835	55.12%	5.616%
57	23.692	3495	3503	3517	rVB	2145512	4589536	94.93%	9.673%
58	23.845	3523	3529	3536	rBV2	1382576	2458806	50.86%	5.182%




Sum of corrected areas: 47447392

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023924.D
Acq On : 03 Feb 2023 02:57
Operator : CG/JU
Sample : 01295-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

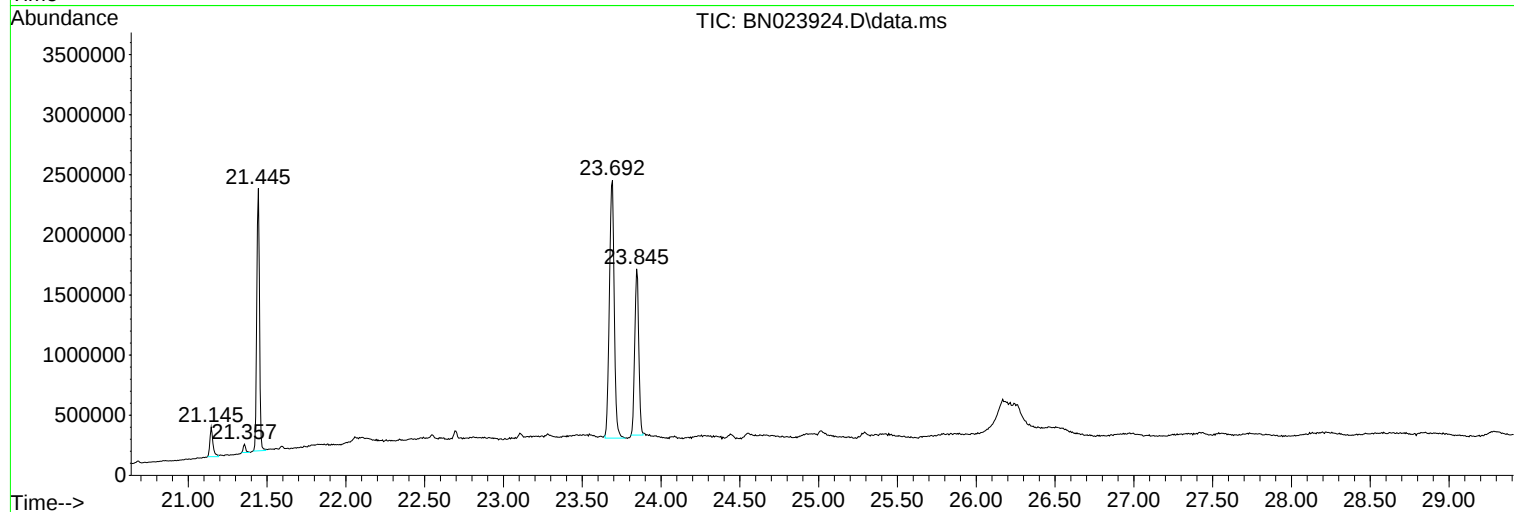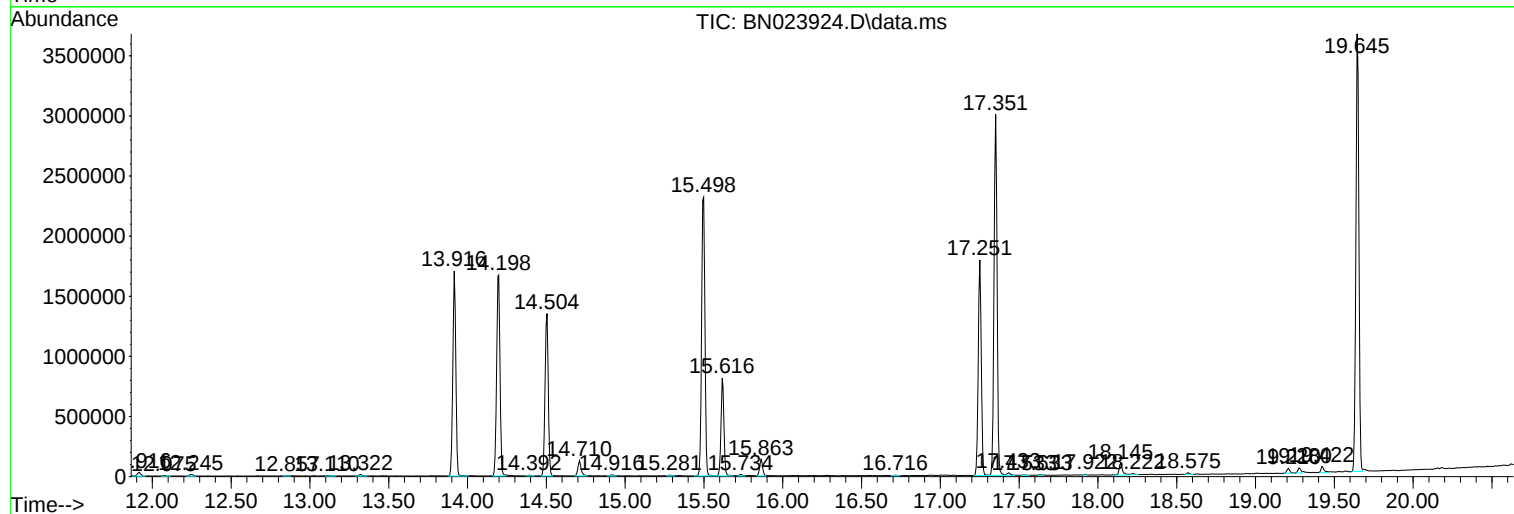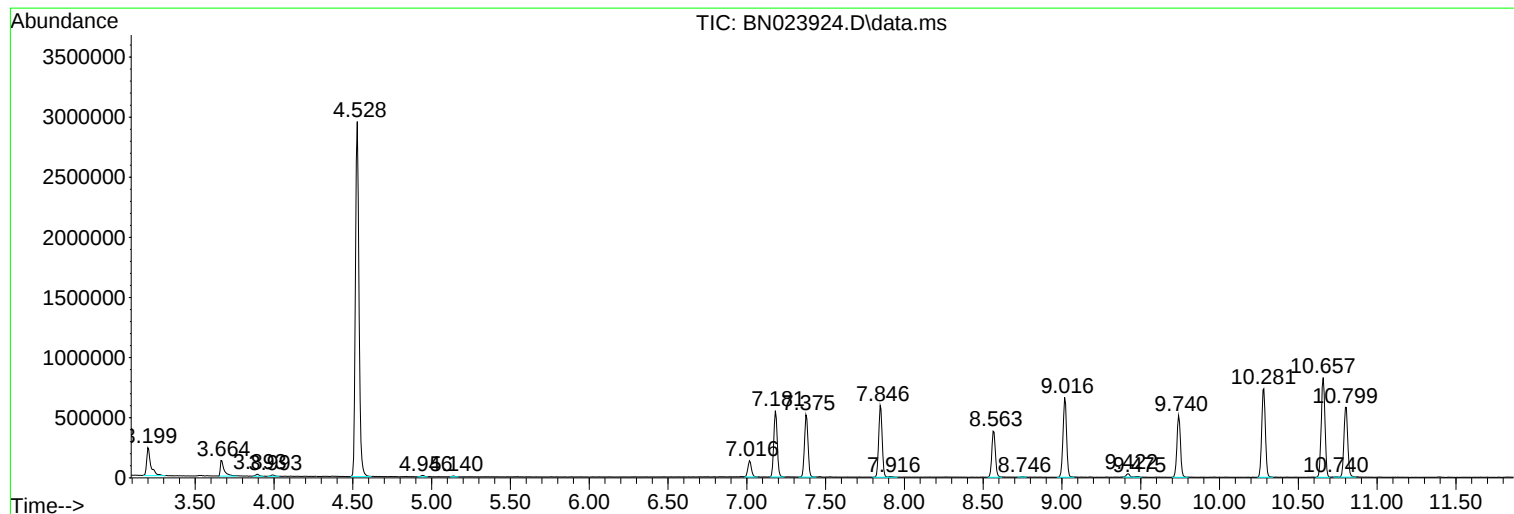

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023924.D
Acq On : 03 Feb 2023 02:57
Operator : CG/JU
Sample : 01295-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dichloroacetic acid, heptad... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.145	2.54 ng/ul	339027	Chrysene-d12	21.445

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2			Pentadecafluorooctanoic acid, he...	638	C24H33F15O2	1000406-04-6	94
3			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
4			Pentacos-1-ene	350	C25H50	016980-85-1	94
5			1-Heneicosanol	312	C21H44O	015594-90-8	93

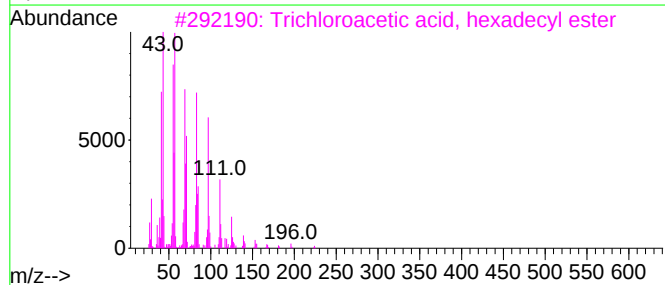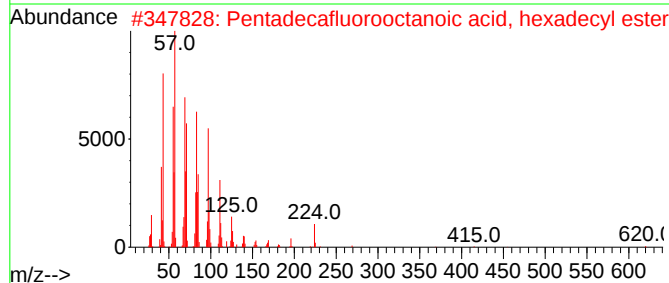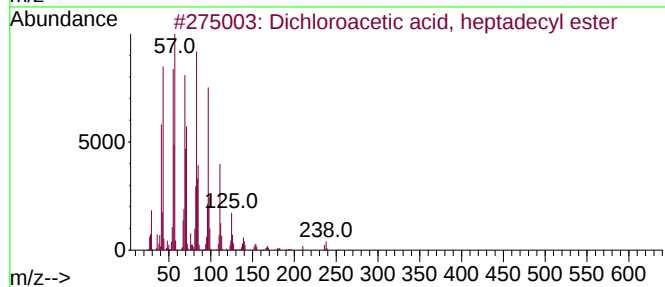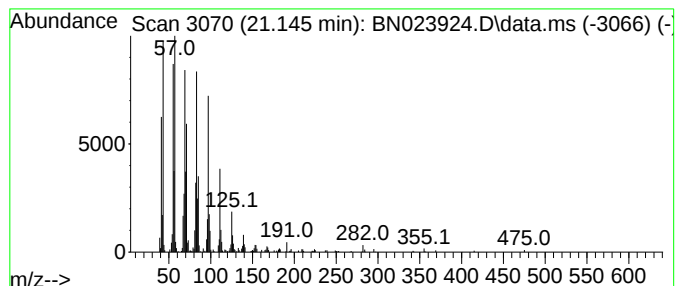

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023924.D
Acq On : 03 Feb 2023 02:57
Operator : CG/JU
Sample : 01295-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	21.145	2.5	ng/u1	339027	5	21.445	2664840	20.0