

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023926.D
 Acq On : 03 Feb 2023 04:10
 Operator : CG/JU
 Sample : 01295-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	32	rVB	32200	43543	0.90%	0.104%
2	3.522	71	74	84	rVB9	4749	9888	0.21%	0.024%
3	3.664	95	98	111	rBV	156995	251782	5.22%	0.600%
4	3.899	132	138	145	rVB	16961	30310	0.63%	0.072%
5	3.993	150	154	158	rVV	11289	14128	0.29%	0.034%
6	4.940	307	315	321	rBV	25672	42027	0.87%	0.100%
7	6.969	656	660	662	rBV3	6937	8510	0.18%	0.020%
8	7.016	662	668	675	rVB	158105	240271	4.98%	0.573%
9	7.181	690	696	704	rBV	579480	861080	17.86%	2.052%
10	7.375	723	729	737	rBV	572119	869616	18.04%	2.073%
11	7.846	803	809	816	rBV	579774	911135	18.90%	2.172%
12	8.099	849	852	858	rVB5	4286	6503	0.13%	0.015%
13	8.563	925	931	940	rBV	415565	658669	13.66%	1.570%
14	9.016	1001	1008	1015	rBV	685671	1076506	22.33%	2.566%
15	9.075	1015	1018	1024	rVB4	23769	36589	0.76%	0.087%
16	9.416	1072	1076	1082	rVB	36411	52755	1.09%	0.126%
17	9.740	1124	1131	1139	rBV	563119	884096	18.34%	2.107%
18	10.281	1212	1223	1232	rBV	793625	1290791	26.77%	3.076%
19	10.587	1271	1275	1280	rBV5	3855	6033	0.13%	0.014%
20	10.657	1280	1287	1300	rBV	837247	1343046	27.86%	3.201%
21	10.798	1304	1311	1321	rBV	709931	1179235	24.46%	2.811%
22	11.569	1438	1442	1446	rBV5	2838	5410	0.11%	0.013%
23	11.610	1446	1449	1455	rVB6	5559	8346	0.17%	0.020%
24	11.916	1494	1501	1507	rVB	40666	62998	1.31%	0.150%
25	12.245	1551	1557	1565	rVB3	15025	25297	0.52%	0.060%
26	12.375	1576	1579	1586	rVB6	4728	7469	0.15%	0.018%
27	12.845	1655	1659	1664	rBV7	3054	5692	0.12%	0.014%
28	13.122	1702	1706	1710	rBV5	3358	5012	0.10%	0.012%
29	13.204	1715	1720	1724	rBV5	2893	5473	0.11%	0.013%
30	13.404	1747	1754	1757	rVB8	2684	5032	0.10%	0.012%
31	13.916	1834	1841	1848	rBV	1740930	2283988	47.38%	5.444%
32	14.198	1882	1889	1899	rBV	1758643	2561138	53.13%	6.104%
33	14.504	1934	1941	1951	rBV	1308674	1895596	39.32%	4.518%
34	14.710	1970	1976	1984	rBV	139755	207353	4.30%	0.494%
35	14.928	2006	2013	2016	rBV7	7061	11928	0.25%	0.028%
36	15.292	2069	2075	2078	rBV6	3396	7000	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023926.D
 Acq On : 03 Feb 2023 04:10
 Operator : CG/JU
 Sample : 01295-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

37	15.492	2101	2109	2122	rVB	2374587	3444320	71.45%	8.209%
38	15.616	2124	2130	2142	rVV	823619	1032774	21.42%	2.462%
39	15.733	2146	2150	2154	rVV3	12631	16136	0.33%	0.038%
40	16.210	2225	2231	2237	rVB7	3306	7304	0.15%	0.017%
41	17.251	2401	2408	2415	rBV	1743148	2361765	48.99%	5.629%
42	17.351	2418	2425	2437	rVV2	2977370	4097047	84.98%	9.765%
43	17.445	2437	2441	2445	rVB3	19091	24331	0.50%	0.058%
44	17.916	2519	2521	2526	rVB5	7151	8013	0.17%	0.019%
45	18.145	2556	2560	2568	rBV7	11496	18950	0.39%	0.045%
46	18.222	2570	2573	2578	rVB4	5320	6269	0.13%	0.015%
47	19.210	2736	2741	2746	rBV	37767	51991	1.08%	0.124%
48	19.280	2748	2753	2757	rBV	37756	51950	1.08%	0.124%
49	19.422	2774	2777	2783	rBV6	11025	18667	0.39%	0.044%
50	19.645	2809	2815	2822	rBV	3713801	4820921	100.00%	11.490%
51	21.345	3102	3104	3108	rVB	54066	51277	1.06%	0.122%
52	21.439	3114	3120	3125	rBV	1924190	2490283	51.66%	5.935%
53	23.668	3491	3499	3511	rBV2	2149590	4262934	88.43%	10.160%
54	23.821	3518	3525	3536	rVB	1139130	2277311	47.24%	5.428%




Sum of corrected areas: 41956488

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023926.D
Acq On : 03 Feb 2023 04:10
Operator : CG/JU
Sample : 01295-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

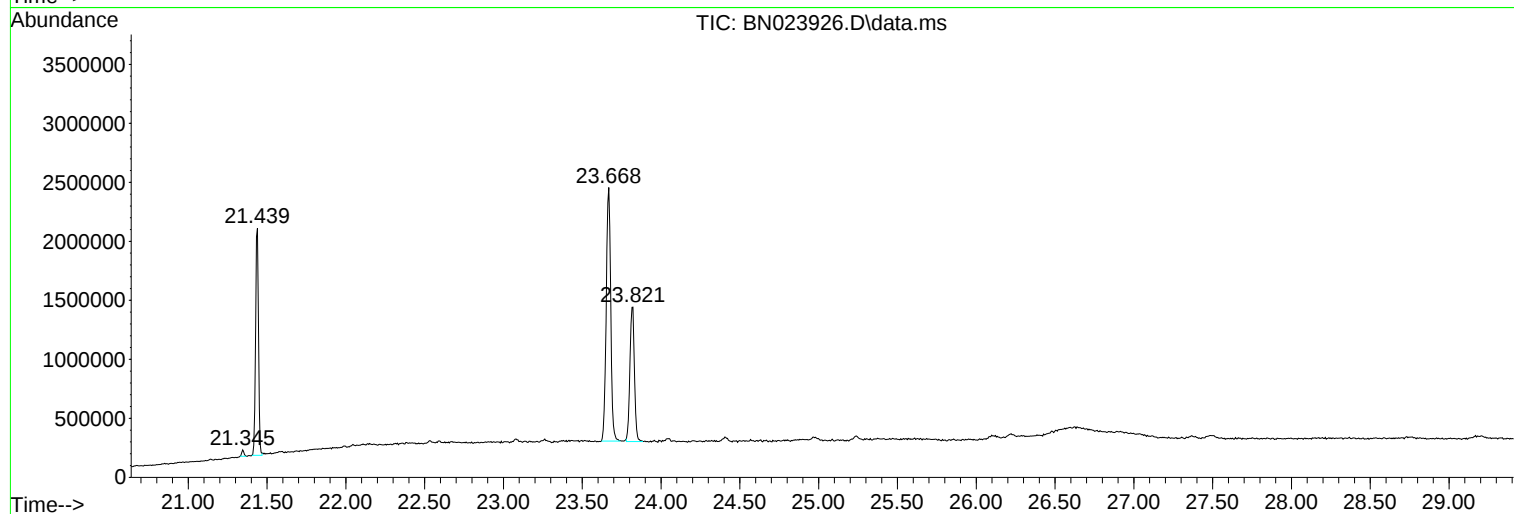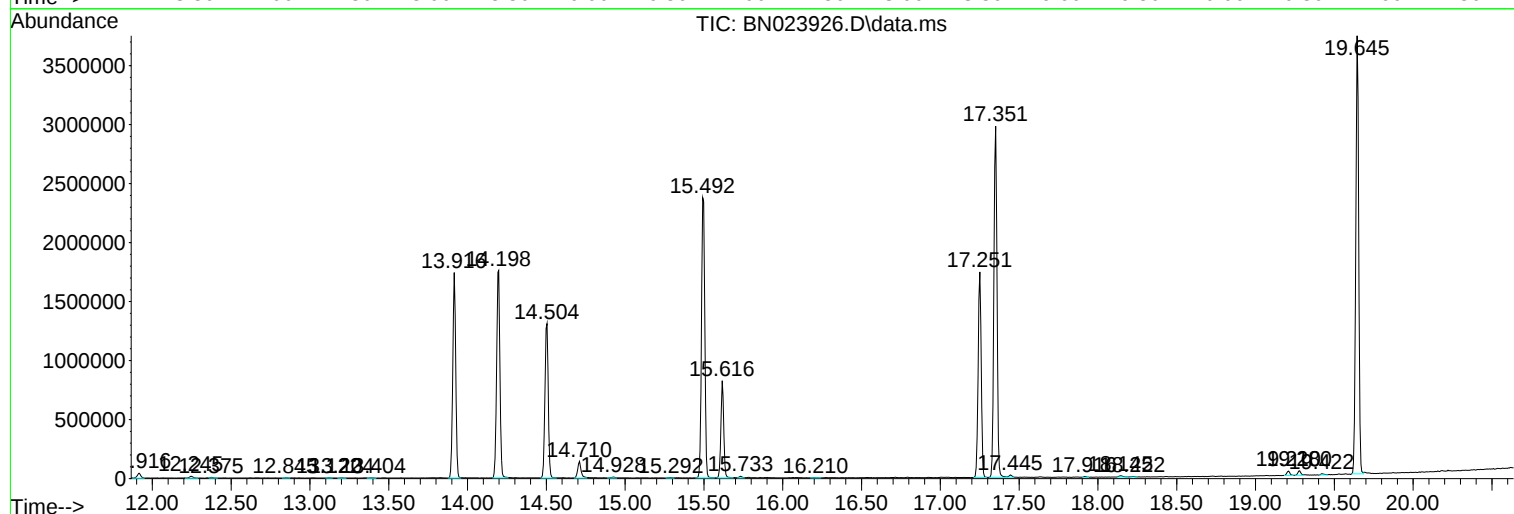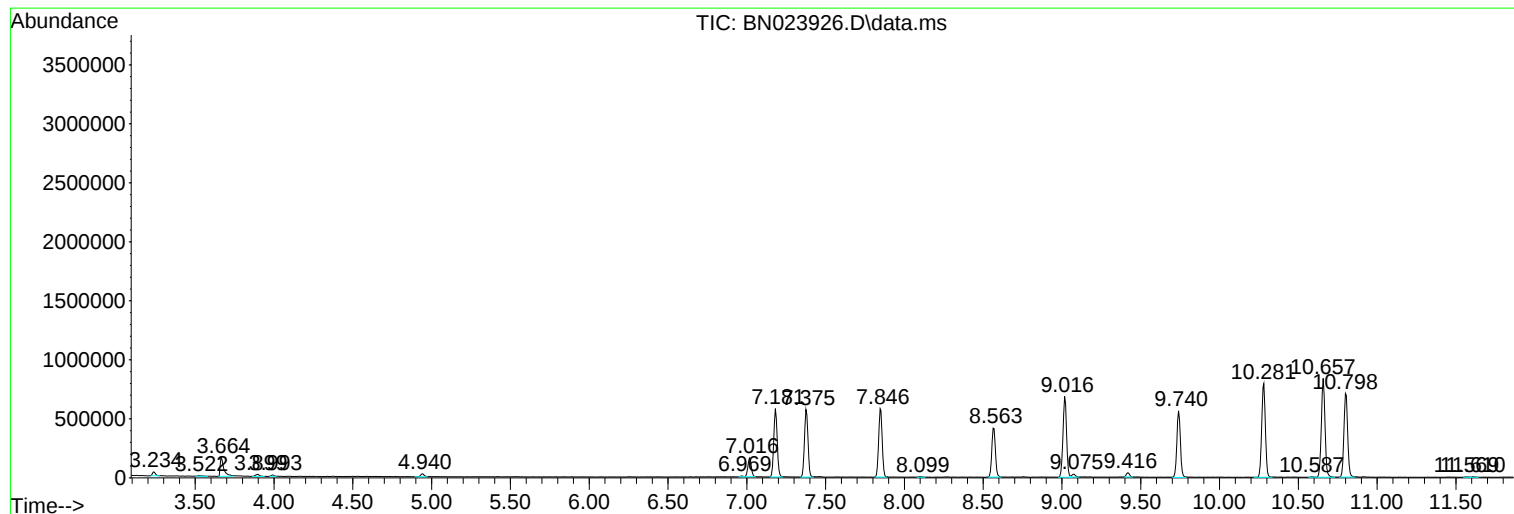

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023926.D
Acq On : 03 Feb 2023 04:10
Operator : CG/JU
Sample : 01295-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023926.D
Acq On : 03 Feb 2023 04:10
Operator : CG/JU
Sample : 01295-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc