

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023928.D
 Acq On : 03 Feb 2023 06:00
 Operator : CG/JU
 Sample : PB150527BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK527

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	31	rBV	42861	58785	1.37%	0.128%
2	3.658	94	97	113	rBV	550558	834145	19.42%	1.817%
3	3.993	151	154	161	rVB2	12916	18693	0.44%	0.041%
4	7.016	662	668	677	rBV	735931	1103039	25.67%	2.402%
5	7.181	689	696	707	rBV	592811	882699	20.55%	1.922%
6	7.375	722	729	739	rBV	755611	1153385	26.85%	2.512%
7	7.846	802	809	817	rBV	684870	1045077	24.33%	2.276%
8	8.563	924	931	940	rBV	852837	1375039	32.01%	2.995%
9	9.016	1001	1008	1016	rBV	700742	1104498	25.71%	2.405%
10	9.740	1124	1131	1142	rBV	625613	972583	22.64%	2.118%
11	10.281	1215	1223	1233	rBV	925483	1493390	34.76%	3.252%
12	10.657	1279	1287	1298	rVB	923964	1513592	35.23%	3.296%
13	10.799	1303	1311	1328	rBV	911362	1514092	35.24%	3.297%
14	12.245	1552	1557	1564	rVB	14510	24797	0.58%	0.054%
15	13.916	1834	1841	1851	rBV	1849679	2388767	55.60%	5.202%
16	14.192	1882	1888	1904	rBV	1846981	2657593	61.86%	5.788%
17	14.498	1934	1940	1952	rBV	1484202	2173030	50.58%	4.732%
18	14.710	1969	1976	1995	rBV	818740	1138582	26.50%	2.480%
19	15.287	2069	2074	2080	rVB5	2687	5099	0.12%	0.011%
20	15.492	2101	2109	2119	rBV	2490155	3402923	79.21%	7.411%
21	15.616	2124	2130	2140	rVB	847064	1057961	24.63%	2.304%
22	15.734	2146	2150	2155	rVB2	10165	12803	0.30%	0.028%
23	16.275	2238	2242	2245	rBV4	3718	5461	0.13%	0.012%
24	17.251	2401	2408	2418	rBV	1982189	2684256	62.48%	5.846%
25	17.351	2418	2425	2440	rBV	2619656	3740515	87.07%	8.146%
26	19.210	2736	2741	2746	rBV2	33185	44325	1.03%	0.097%
27	19.275	2749	2752	2757	rVB	29470	38714	0.90%	0.084%
28	19.645	2809	2815	2821	rBV	3356616	4296228	100.00%	9.356%
29	21.351	3103	3105	3109	rBV	36152	42418	0.99%	0.092%
30	21.445	3115	3121	3129	rBV	2179501	2747074	63.94%	5.983%
31	23.680	3494	3501	3515	rVB2	1881019	3888830	90.52%	8.469%
32	23.845	3522	3529	3539	rBV2	1355179	2499917	58.19%	5.444%




Sum of corrected areas: 45918310

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023928.D
Acq On : 03 Feb 2023 06:00
Operator : CG/JU
Sample : PB150527BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

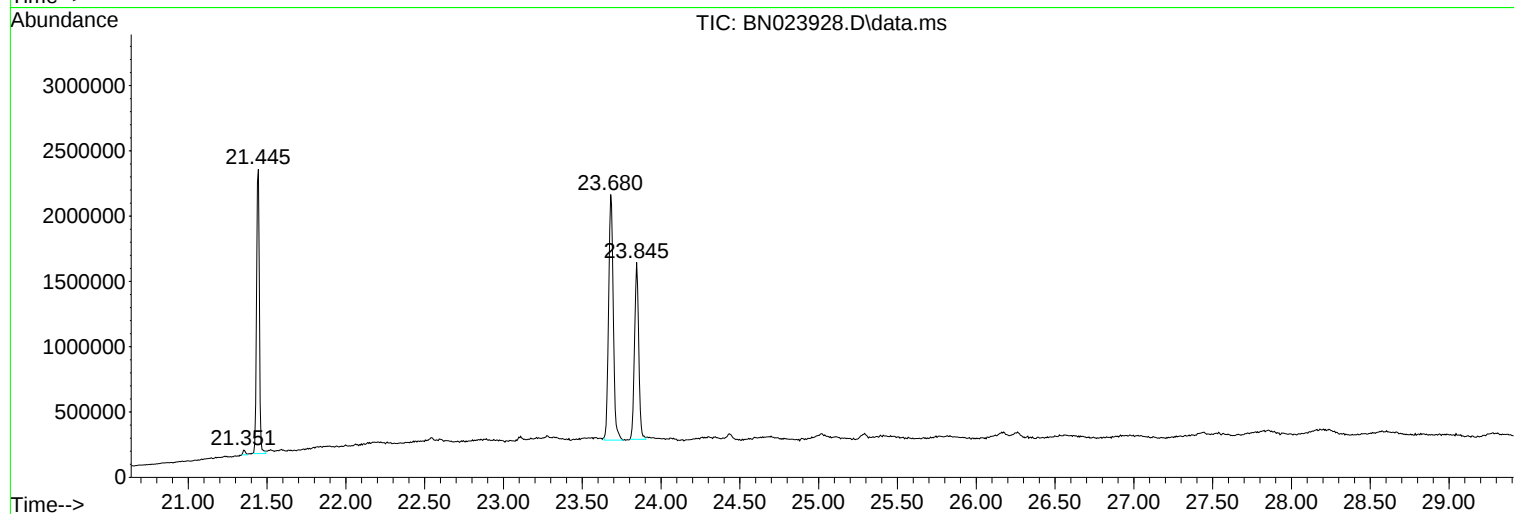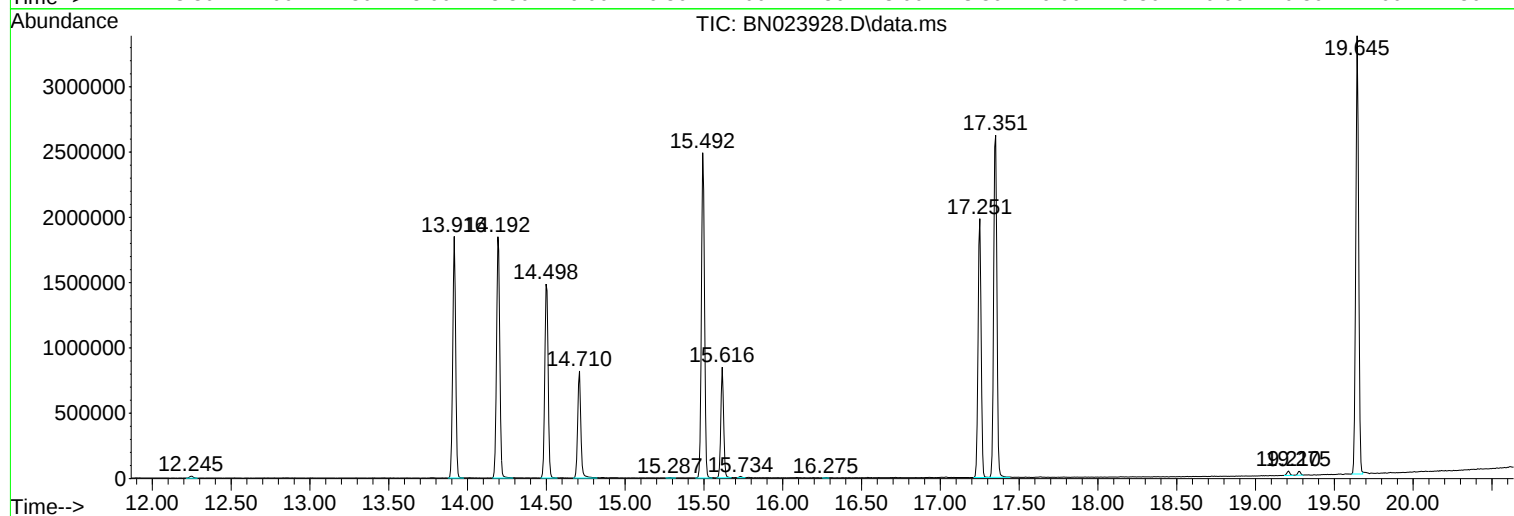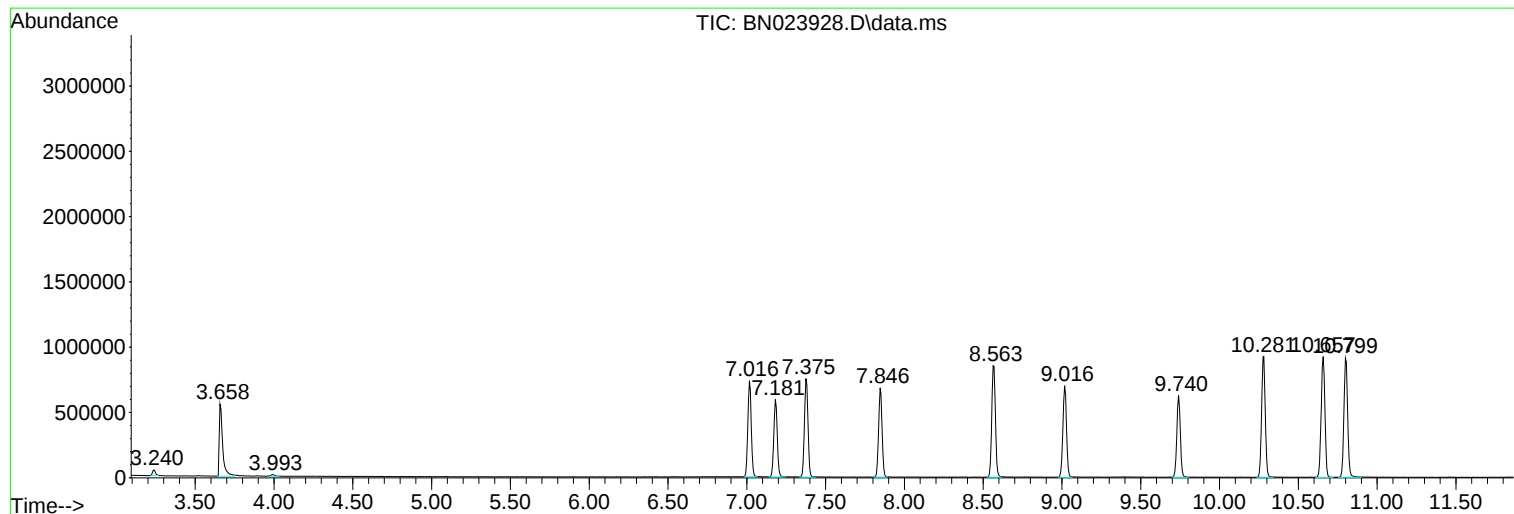

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023928.D
Acq On : 03 Feb 2023 06:00
Operator : CG/JU
Sample : PB150527BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023928.D
Acq On : 03 Feb 2023 06:00
Operator : CG/JU
Sample : PB150527BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc