

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023934.D
 Acq On : 03 Feb 2023 09:39
 Operator : CG/JU
 Sample : 01294-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	29	rBV	45934	64413	1.29%	0.131%
2	3.270	29	31	40	rVB	55864	77734	1.56%	0.158%
3	3.658	94	97	120	rBV	604845	910904	18.22%	1.853%
4	3.893	133	137	142	rVB	13087	18343	0.37%	0.037%
5	3.940	142	145	148	rVB4	5466	5410	0.11%	0.011%
6	3.993	149	154	161	rVB	39483	60033	1.20%	0.122%
7	6.928	649	653	656	rBV3	6374	8495	0.17%	0.017%
8	7.017	660	668	675	rBV	847475	1275620	25.52%	2.595%
9	7.181	689	696	709	rBV	687777	1023399	20.47%	2.082%
10	7.375	722	729	737	rBV	864854	1298251	25.97%	2.641%
11	7.464	740	744	745	rVV2	4175	5913	0.12%	0.012%
12	7.487	745	748	754	rVB2	8095	12951	0.26%	0.026%
13	7.846	802	809	817	rVB	572099	864551	17.30%	1.759%
14	7.958	825	828	833	rVB4	3971	5935	0.12%	0.012%
15	8.564	924	931	944	rBV	1037931	1624915	32.51%	3.305%
16	9.016	1000	1008	1020	rBV	824247	1279855	25.60%	2.604%
17	9.740	1121	1131	1145	rBV	747006	1185112	23.71%	2.411%
18	10.275	1215	1222	1237	rBV	1104492	1761489	35.24%	3.583%
19	10.658	1279	1287	1295	rBV	751766	1259149	25.19%	2.561%
20	10.799	1304	1311	1327	rBV	1011786	1762593	35.26%	3.586%
21	12.246	1547	1557	1563	rBV2	18209	31365	0.63%	0.064%
22	13.916	1834	1841	1849	rBV	2131125	2794184	55.90%	5.684%
23	14.193	1881	1888	1901	rBV	2221881	3157424	63.17%	6.423%
24	14.499	1933	1940	1949	rBV	1273648	1803741	36.09%	3.669%
25	14.710	1969	1976	1992	rBV	965875	1347238	26.95%	2.741%
26	14.922	2006	2012	2020	rVB3	25637	41104	0.82%	0.084%
27	15.493	2100	2109	2122	rBV	2925382	4038005	80.78%	8.214%
28	15.616	2124	2130	2138	rBV	1057190	1329797	26.60%	2.705%
29	15.734	2146	2150	2155	rBV2	12915	19102	0.38%	0.039%
30	16.269	2237	2241	2250	rBV8	2275	5481	0.11%	0.011%
31	16.716	2313	2317	2324	rBV6	2556	5029	0.10%	0.010%
32	17.245	2401	2407	2416	rBV	1535582	2193993	43.89%	4.463%
33	17.351	2418	2425	2438	rVV	3111651	4363126	87.29%	8.876%
34	17.445	2438	2441	2446	rVB6	13908	18224	0.36%	0.037%
35	17.634	2471	2473	2477	rVB4	4166	5047	0.10%	0.010%
36	17.922	2519	2522	2528	rVB5	4607	6445	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023934.D
 Acq On : 03 Feb 2023 09:39
 Operator : CG/JU
 Sample : 01294-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

37	18.145	2557	2560	2564	rVB5	5588	6228	0.12%	0.013%
38	19.204	2736	2740	2746	rVB2	37470	51810	1.04%	0.105%
39	19.281	2748	2753	2759	rBV	36548	53491	1.07%	0.109%
40	19.569	2799	2802	2805	rBV5	7921	9048	0.18%	0.018%
41	19.645	2809	2815	2822	rBV	3737059	4998525	100.00%	10.168%
42	21.445	3116	3121	3127	rBV	1836921	2189796	43.81%	4.455%
43	23.680	3494	3501	3514	rVB2	2138204	4317510	86.38%	8.783%
44	23.845	3522	3529	3537	rBV2	915752	1867162	37.35%	3.798%




Sum of corrected areas: 49157940

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023934.D
Acq On : 03 Feb 2023 09:39
Operator : CG/JU
Sample : 01294-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

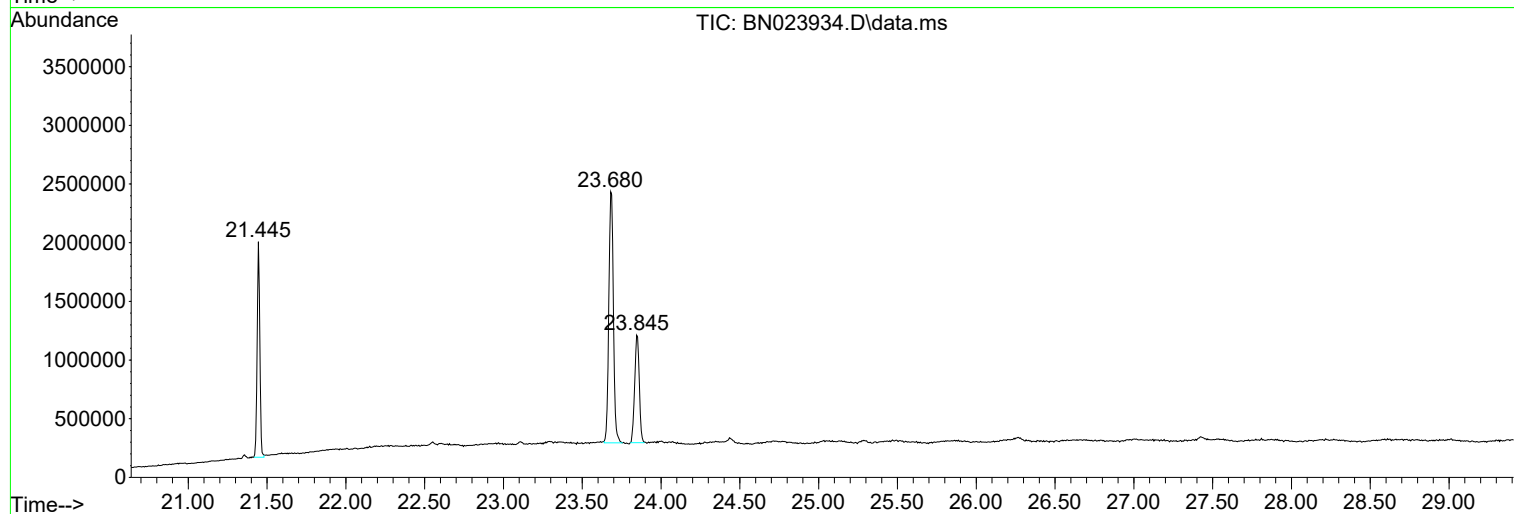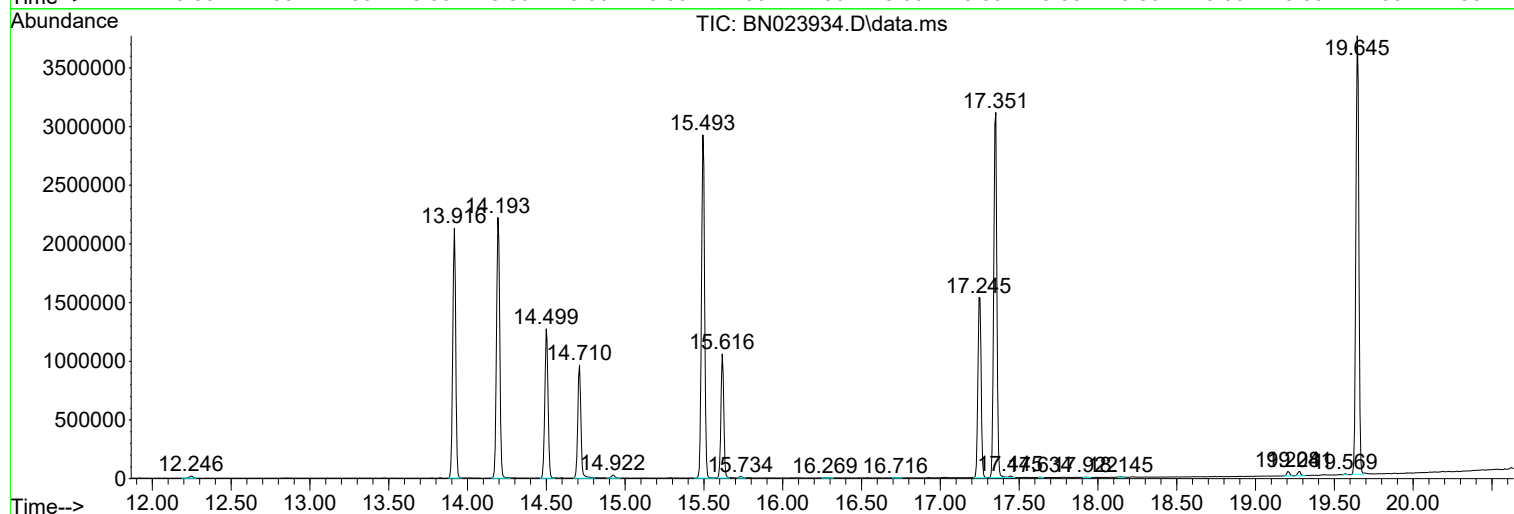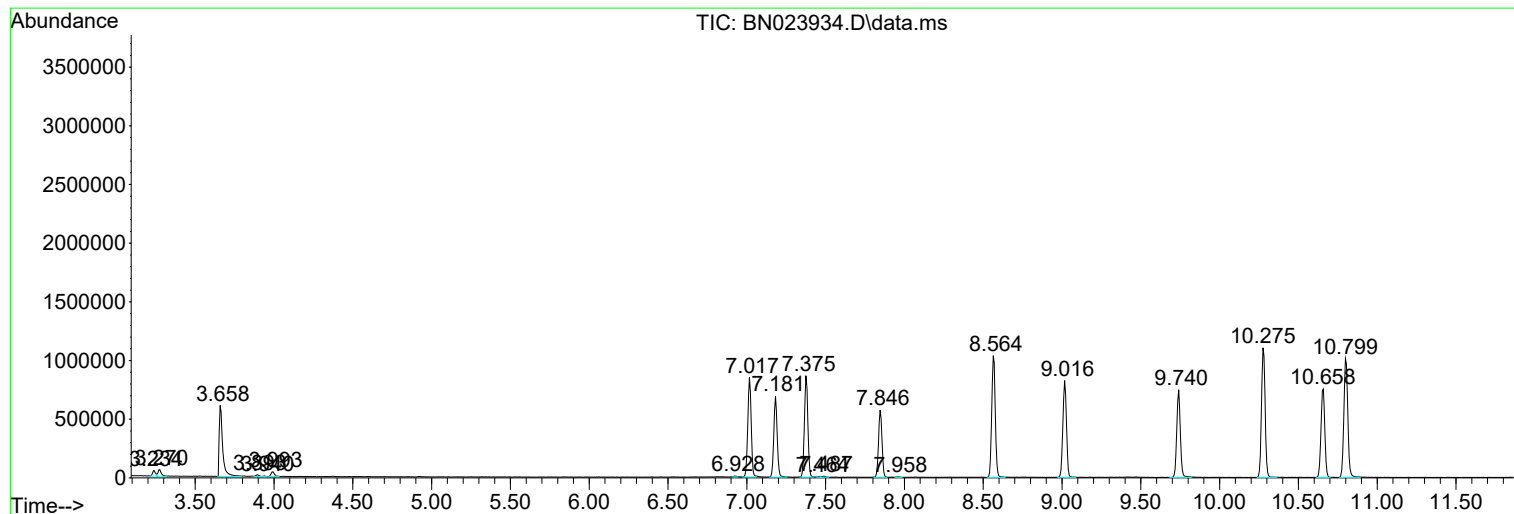

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023934.D
Acq On : 03 Feb 2023 09:39
Operator : CG/JU
Sample : 01294-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023934.D
Acq On : 03 Feb 2023 09:39
Operator : CG/JU
Sample : 01294-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44P8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------