

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
 Data File : BN023936.D
 Acq On : 03 Feb 2023 10:52
 Operator : CG/JU
 Sample : PB150528BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	32	rVB	42341	57232	1.38%	0.132%
2	3.658	94	97	119	rBV	548814	832722	20.08%	1.914%
3	3.993	150	154	159	rVB	10788	17179	0.41%	0.039%
4	7.016	661	668	680	rVB	732258	1081053	26.07%	2.484%
5	7.181	690	696	707	rVB	592849	867341	20.92%	1.993%
6	7.375	723	729	739	rBV	748625	1118834	26.98%	2.571%
7	7.846	802	809	818	rBV	629072	952820	22.98%	2.190%
8	8.563	924	931	940	rBV	857524	1342683	32.38%	3.086%
9	9.016	999	1008	1017	rBV	700641	1091406	26.32%	2.508%
10	9.740	1123	1131	1143	rBV	622365	965438	23.28%	2.219%
11	10.275	1215	1222	1235	rBV	901218	1465944	35.35%	3.369%
12	10.657	1279	1287	1297	rBV	869431	1406624	33.92%	3.233%
13	10.799	1304	1311	1325	rBV	897964	1479198	35.67%	3.400%
14	12.246	1553	1557	1566	rVB3	13748	23170	0.56%	0.053%
15	13.398	1749	1753	1759	rVB3	9985	15222	0.37%	0.035%
16	13.916	1834	1841	1851	rBV	1805129	2331197	56.22%	5.358%
17	14.193	1881	1888	1899	rBV	1860791	2628358	63.39%	6.041%
18	14.498	1934	1940	1949	rBV	1404701	2017519	48.66%	4.637%
19	14.710	1969	1976	1995	rBV	767663	1103143	26.60%	2.535%
20	15.275	2069	2072	2077	rBV6	2854	5363	0.13%	0.012%
21	15.492	2102	2109	2122	rBV	2415013	3320296	80.07%	7.631%
22	15.616	2124	2130	2141	rVV	842938	1044979	25.20%	2.402%
23	15.734	2144	2150	2154	rBV2	12317	16380	0.40%	0.038%
24	17.251	2401	2408	2418	rBV	1754022	2463042	59.40%	5.661%
25	17.345	2418	2424	2437	rBV	2551378	3645201	87.91%	8.377%
26	17.634	2469	2473	2478	rBV6	3990	5071	0.12%	0.012%
27	19.210	2736	2741	2746	rVB3	30520	41654	1.00%	0.096%
28	19.275	2748	2752	2759	rVV	29153	40734	0.98%	0.094%
29	19.645	2809	2815	2822	rBV	3252778	4146573	100.00%	9.530%
30	21.445	3116	3121	3127	rBV	1931794	2384501	57.51%	5.480%
31	23.686	3495	3502	3517	rVB	1679464	3525183	85.01%	8.102%
32	23.845	3523	3529	3537	rVB	1137818	2075876	50.06%	4.771%




Sum of corrected areas: 43511936

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023936.D
Acq On : 03 Feb 2023 10:52
Operator : CG/JU
Sample : PB150528BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

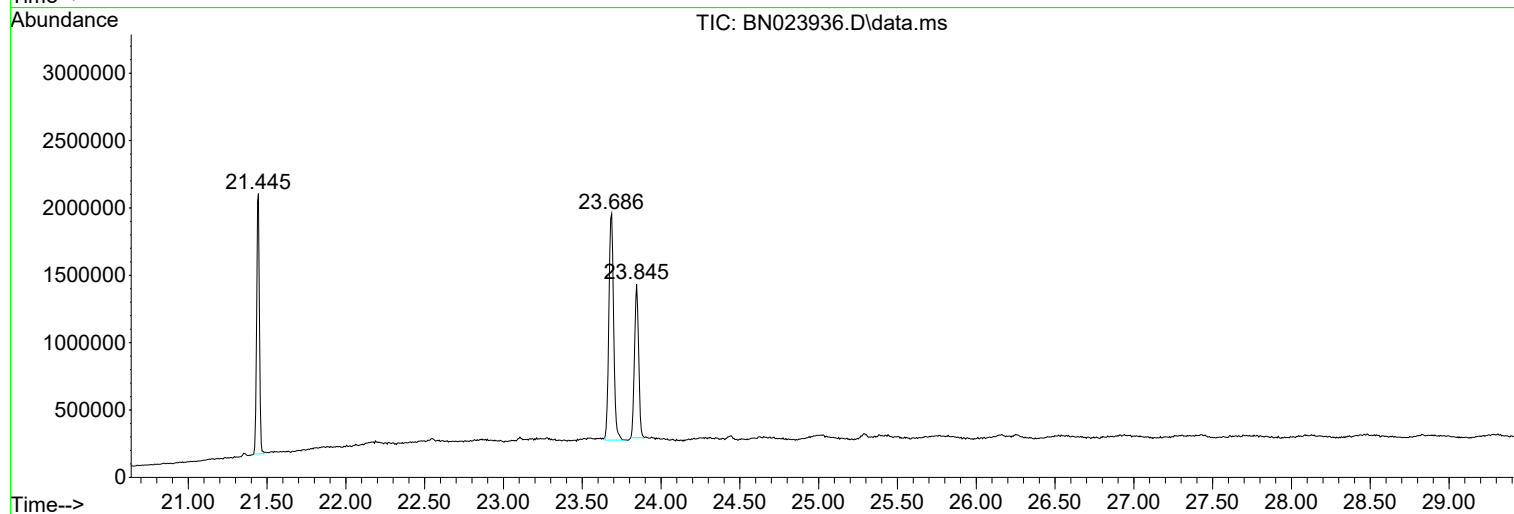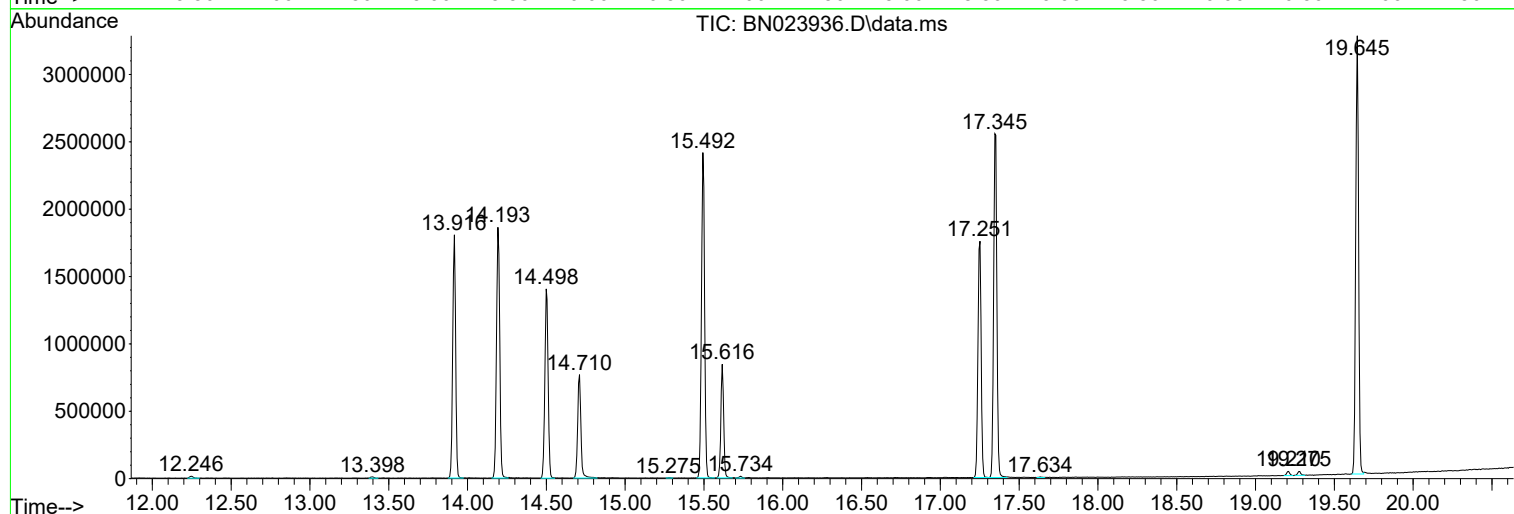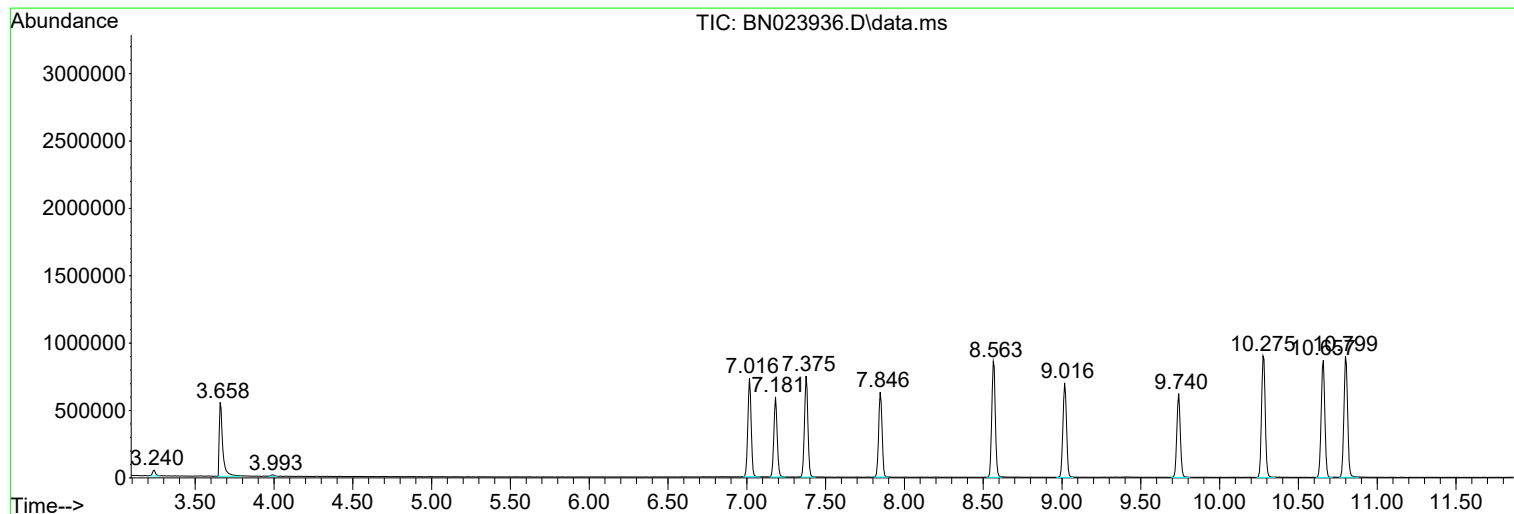

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023936.D
Acq On : 03 Feb 2023 10:52
Operator : CG/JU
Sample : PB150528BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020223\
Data File : BN023936.D
Acq On : 03 Feb 2023 10:52
Operator : CG/JU
Sample : PB150528BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020123.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------