

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023955.D
 Acq On : 06 Feb 2023 16:35
 Operator : CG/JU
 Sample : 01362-05ME
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4443ME

Quant Time: Feb 07 03:00:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 07 02:28:26 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	158958	20.000	ng/ul	0.00
20) Naphthalene-d8	10.646	136	648390	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.493	164	387797	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	841610	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	610152	20.000	ng/ul	0.00
88) Perylene-d12	23.822	264	672872	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	19107	4.861	ng/uL	0.00
4) Pyridine-d5	3.652	84	225757	20.703	ng/ul	0.00
7) Phenol-d5	7.011	99	361268	26.586	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	239932	27.980	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	295582	27.967	ng/ul	0.00
15) 4-Methylphenol-d8	8.558	113	292004	27.506	ng/ul	0.00
21) Nitrobenzene-d5	9.011	128	146696	28.340	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	167439	28.809	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	297224	27.442	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	403268	27.549	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	880329	29.371	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	996361	30.006	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	128416	24.907	ng/ul	0.00
60) Fluorene-d10	15.487	176	735426	29.141	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	120685	20.755	ng/ul	0.00
73) Anthracene-d10	17.351	188	1022182	26.662	ng/ul	0.01
81) Pyrene-d10	19.639	212	1121314	30.508	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	1076625	31.275	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.363	149	10404480	402.045	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023955.D
Acq On : 06 Feb 2023 16:35
Operator : CG/JU
Sample : 01362-05ME
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4443ME

Quant Time: Feb 07 03:00:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 07 02:28:26 2023
Response via : Initial Calibration

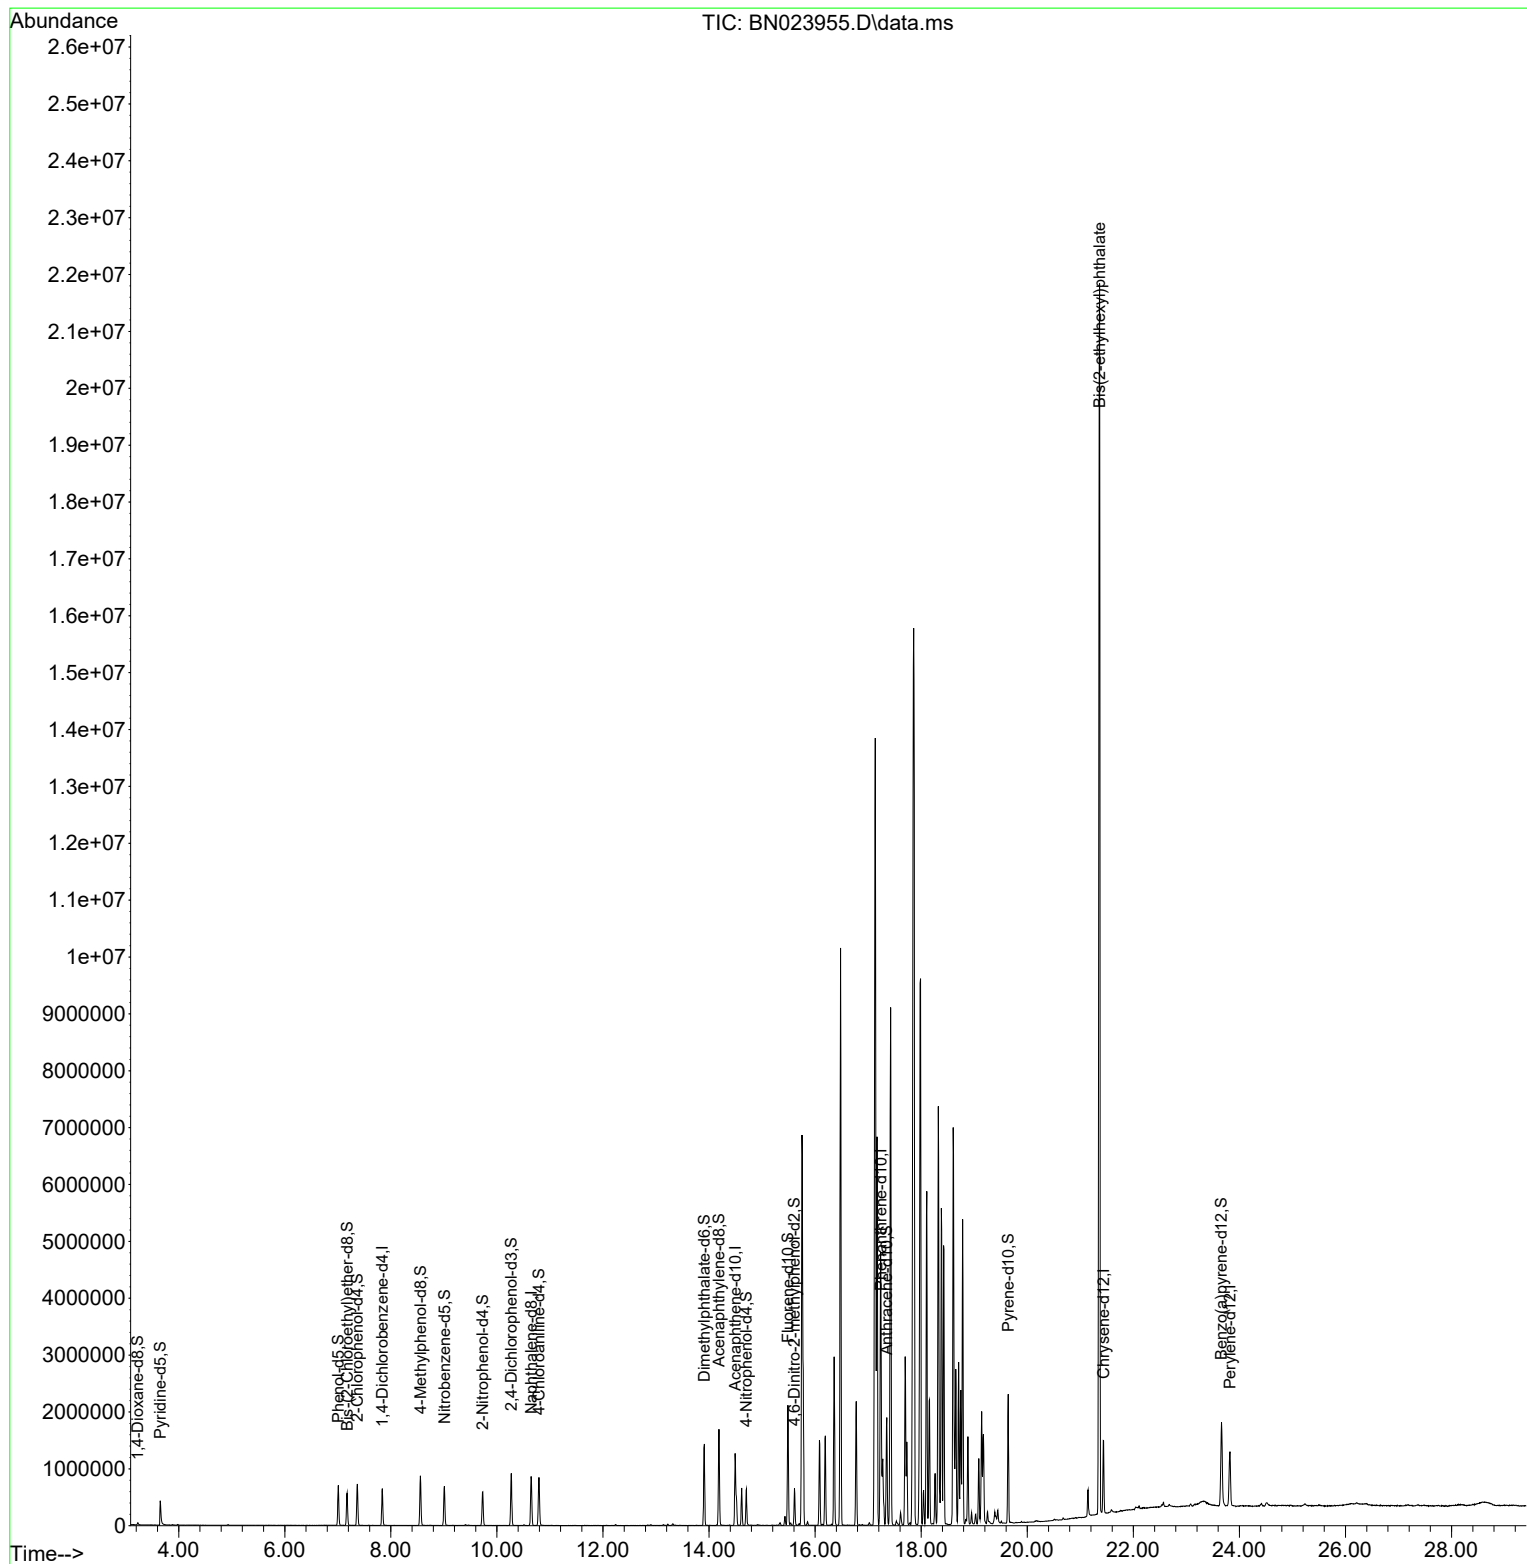

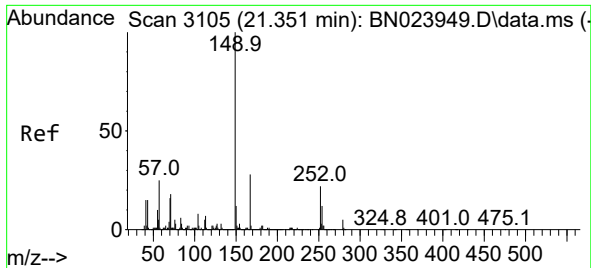

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 402.045 ng/ul
 RT: 21.363 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BN023955.D
 Acq: 06 Feb 2023 16:35

Instrument :
 BNA_N
 ClientSampleId :
 A4443ME

Tgt Ion:149 Resp:10404480
 Ion Ratio Lower Upper
 149 100
 167 31.0 22.7 34.1
 279 9.1 3.9 5.9#

