

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023957.D
 Acq On : 06 Feb 2023 17:48
 Operator : CG/JU
 Sample : 01362-12MEDL 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4488MEDL

Quant Time: Feb 07 03:01:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 07 02:28:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	139533	20.000	ng/ul	0.00
20) Naphthalene-d8	10.646	136	582167	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.493	164	384523	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188	848159	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	700635	20.000	ng/ul	0.00
88) Perylene-d12	23.827	264	721758	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	810	0.235	ng/uL	0.00
4) Pyridine-d5	3.634	84	192	0.020	ng/ul	-0.02
7) Phenol-d5	7.011	99	6192	0.519	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	4809	0.639	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	5212	0.562	ng/ul	0.00
15) 4-Methylphenol-d8	8.558	113	4607	0.494	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	2318	0.499	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	2261	0.433	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	4814	0.495	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	7112	0.541	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	18468	0.621	ng/ul	0.00
49) Acenaphthylene-d8	14.187	160	17699	0.538	ng/ul	0.00
54) 4-Nitrophenol-d4	14.710	143	1257	0.246	ng/ul	0.00
60) Fluorene-d10	15.487	176	17463	0.698	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	1186	0.202	ng/ul	0.00
73) Anthracene-d10	17.339	188	24558	0.636	ng/ul	0.00
81) Pyrene-d10	19.639	212	27697	0.656	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	22865	0.619	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.351	149	4209078	141.640	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023957.D
Acq On : 06 Feb 2023 17:48
Operator : CG/JU
Sample : 01362-12MEDL 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4488MEDL

Quant Time: Feb 07 03:01:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 07 02:28:26 2023
Response via : Initial Calibration

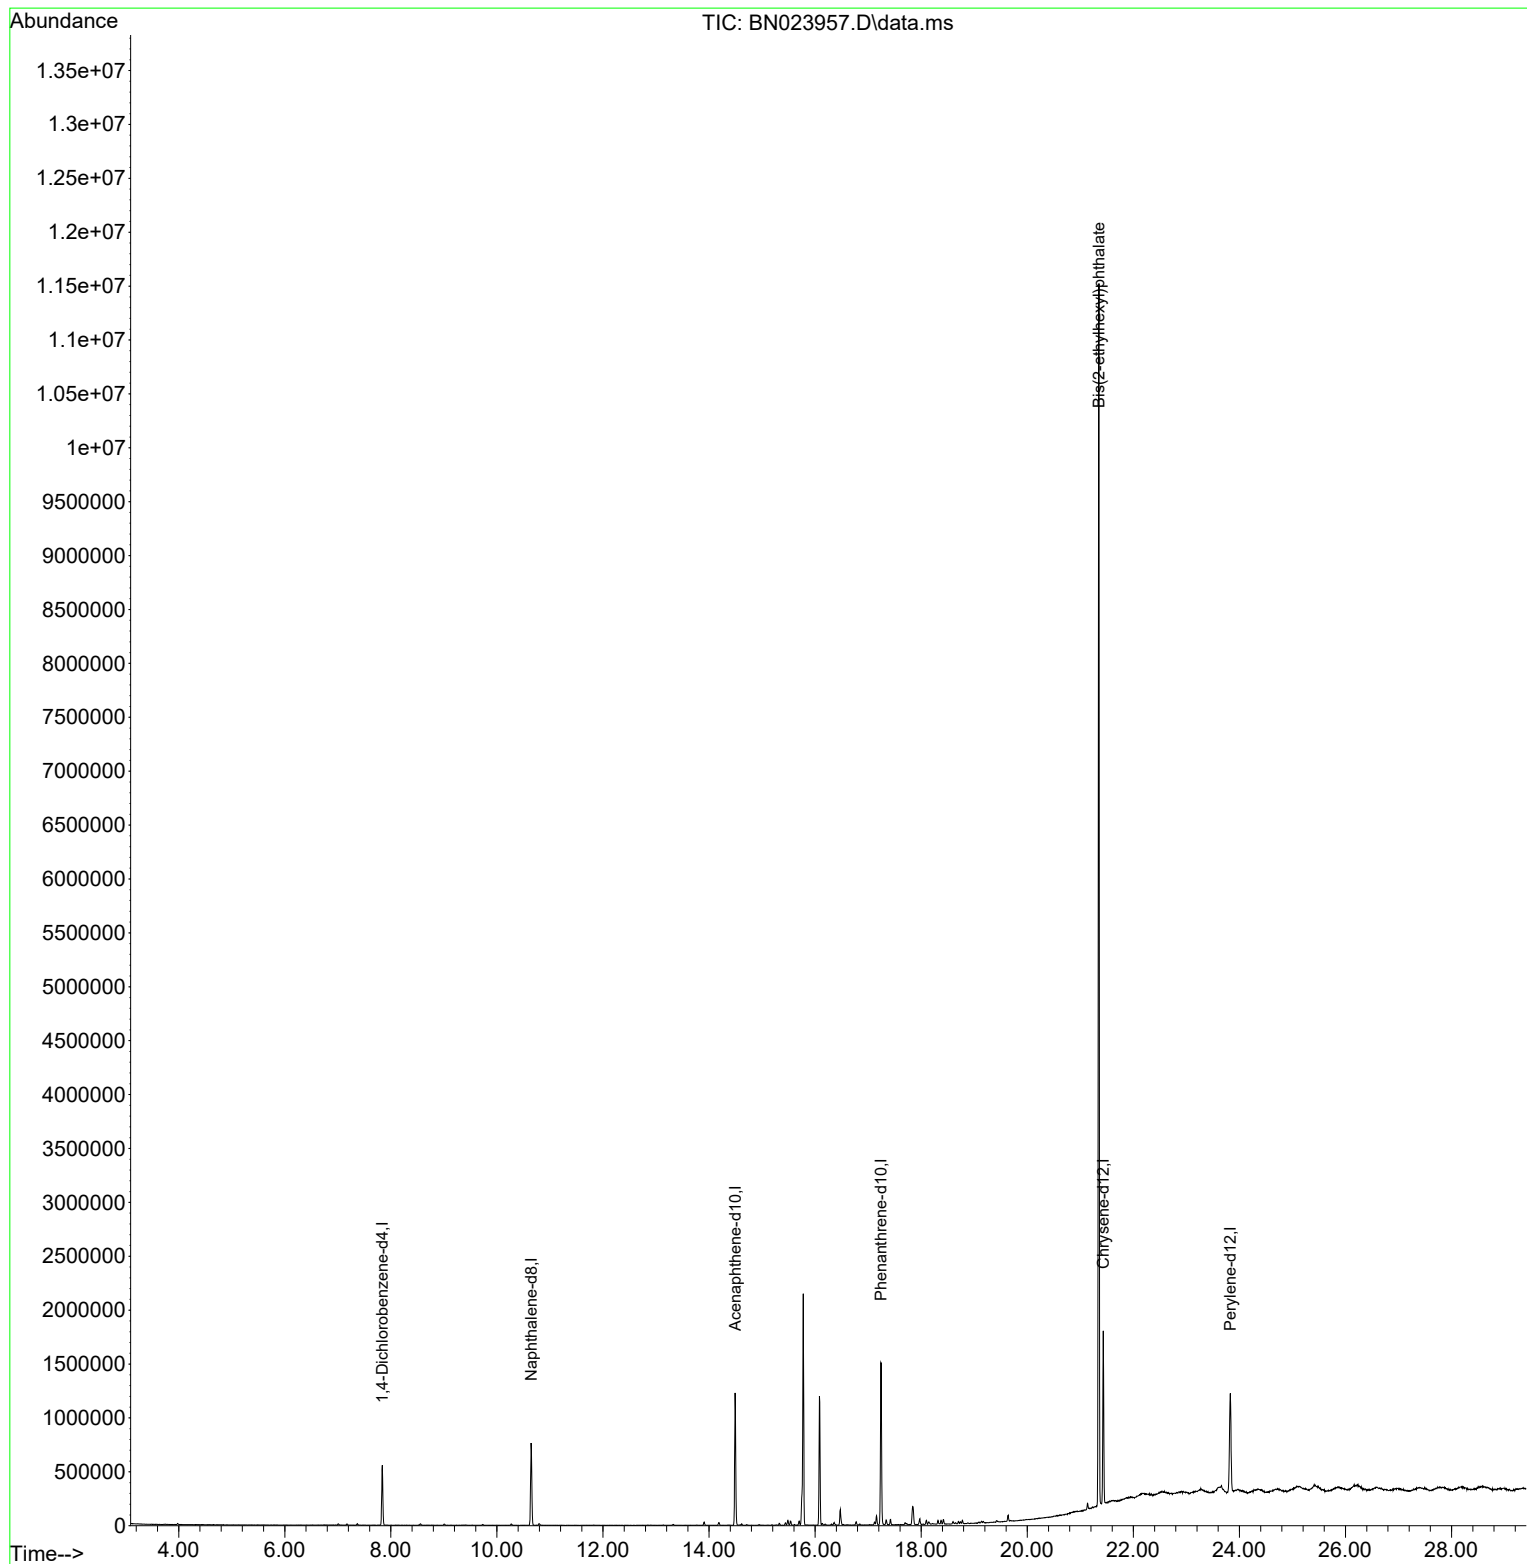

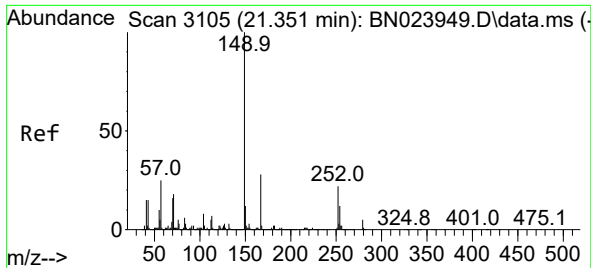

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 141.640 ng/ul
 RT: 21.351 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN023957.D
 Acq: 06 Feb 2023 17:48

Instrument :
 BNA_N
 ClientSampleId :
 A4488MEDL

Tgt Ion:149 Resp: 4209078
 Ion Ratio Lower Upper
 149 100
 167 28.1 22.7 34.1
 279 5.1 3.9 5.9

