

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023956.D
 Acq On : 06 Feb 2023 17:11
 Operator : CG/JU
 Sample : 01362-12ME
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4488ME

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2023
 Supervised By :mohammad ahmed 02/07/2023

Quant Time: Feb 07 03:01:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 07 02:28:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	162643	20.000	ng/u1	0.00
20) Naphthalene-d8	10.646	136	667593	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.493	164	422251	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.245	188	849800	20.000	ng/u1	0.00
79) Chrysene-d12	21.445	240	377418	20.000	ng/u1	0.00
88) Perylene-d12	23.839	264	662543	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	19755	4.912	ng/uL	0.00
4) Pyridine-d5	3.652	84	253203	22.694	ng/u1	0.00
7) Phenol-d5	7.011	99	428973	30.853	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	270548	30.835	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	341448	31.575	ng/u1	0.00
15) 4-Methylphenol-d8	8.558	113	346378	31.889	ng/u1	0.00
21) Nitrobenzene-d5	9.011	128	170164	31.929	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	191778	32.047	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	351088	31.482	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	470015	31.185	ng/u1	0.00
46) Dimethylphthalate-d6	13.910	166	1054617	32.315	ng/u1	0.00
49) Acenaphthylene-d8	14.187	160	1163866	32.191	ng/u1	0.00
54) 4-Nitrophenol-d4	14.704	143	158342	28.205	ng/u1	0.00
60) Fluorene-d10	15.487	176	881401	32.076	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	144364	24.588	ng/u1	0.02
73) Anthracene-d10	17.345	188	1232677	31.843	ng/u1	0.00
81) Pyrene-d10	19.639	212	1308909	57.573	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1128641	33.297	ng/u1	0.00

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.380	149	42951136m	2683.146	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023956.D
Acq On : 06 Feb 2023 17:11
Operator : CG/JU
Sample : 01362-12ME
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4488ME

Quant Time: Feb 07 03:01:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 07 02:28:26 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/07/2023
Supervised By :mohammad ahmed 02/07/2023

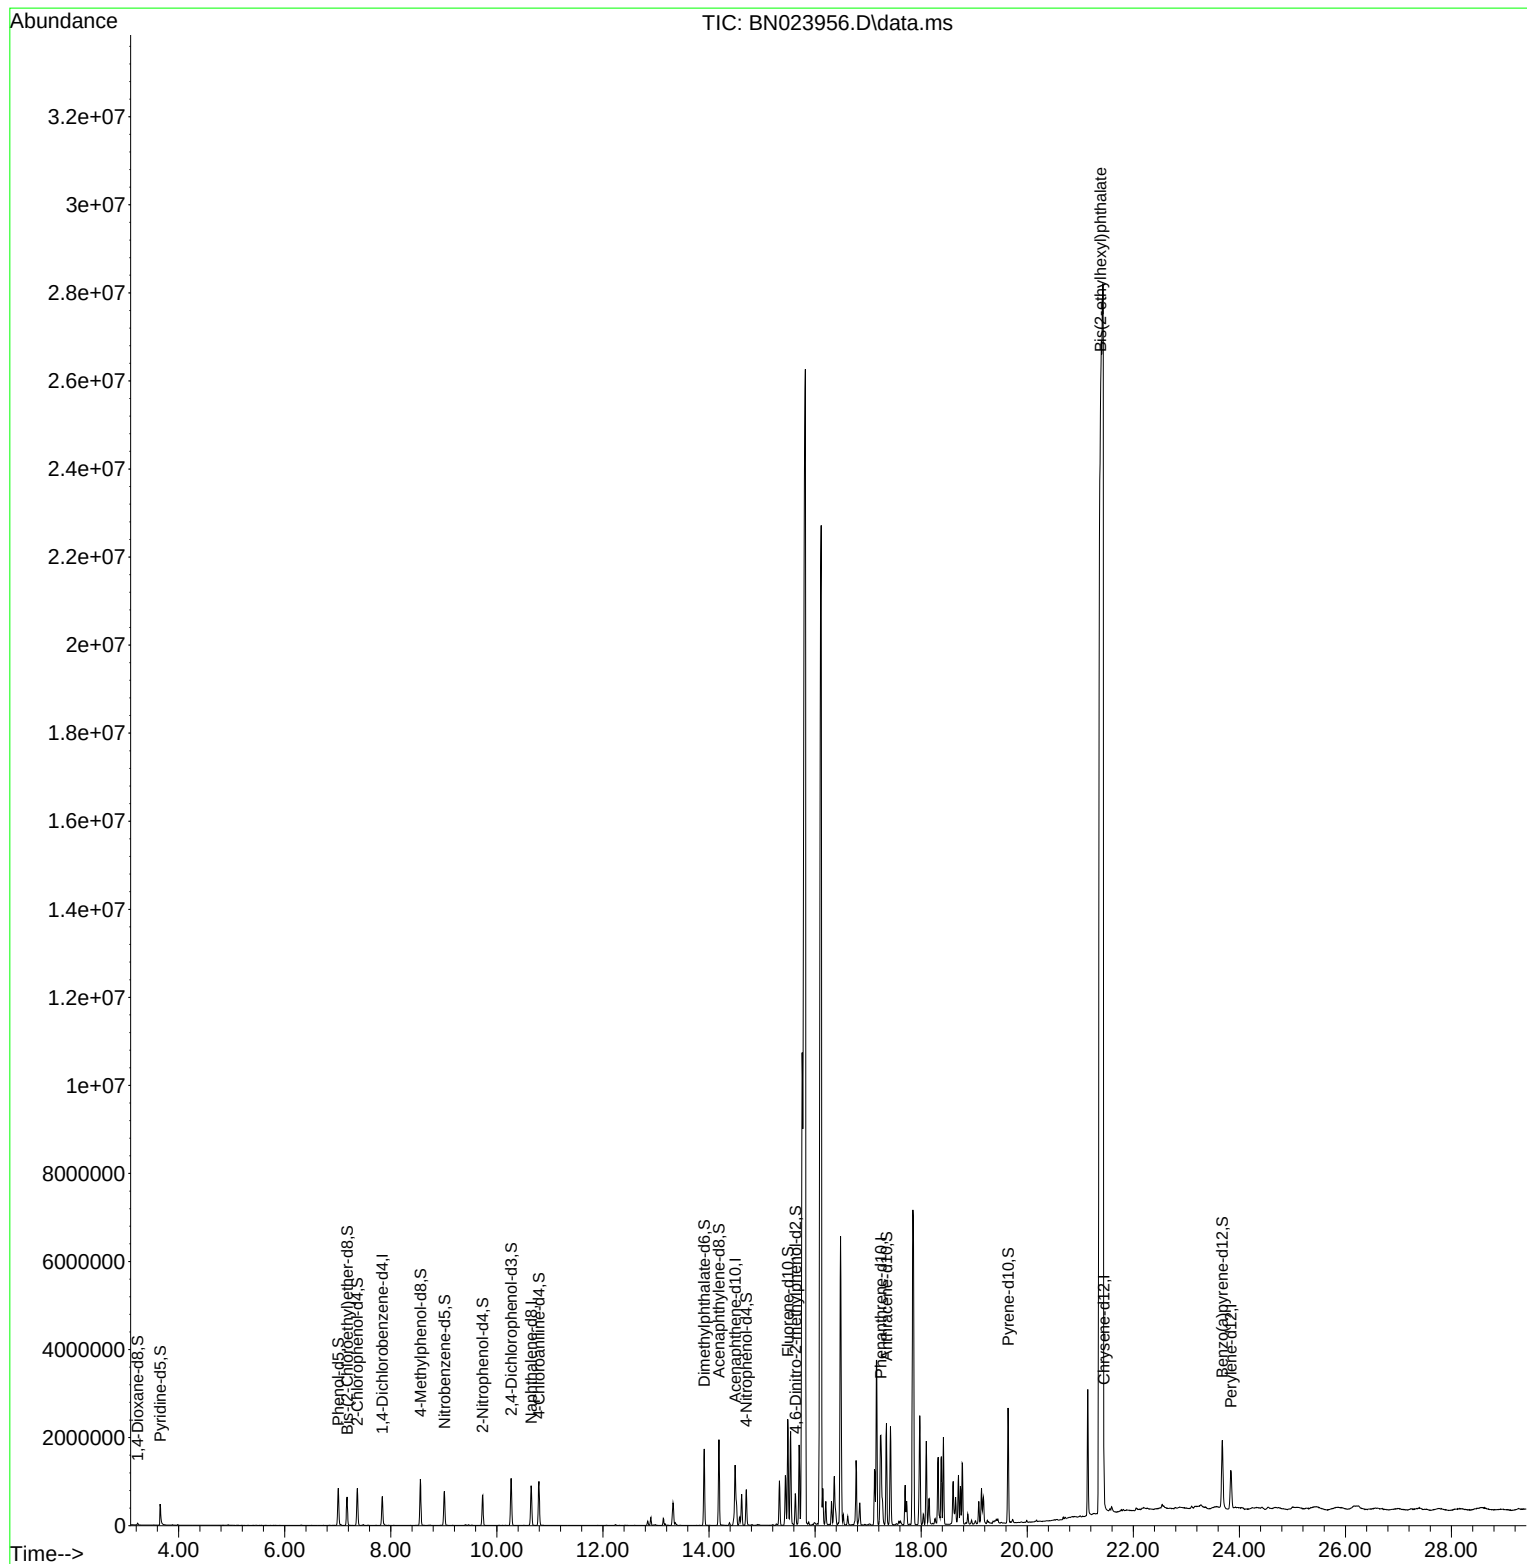

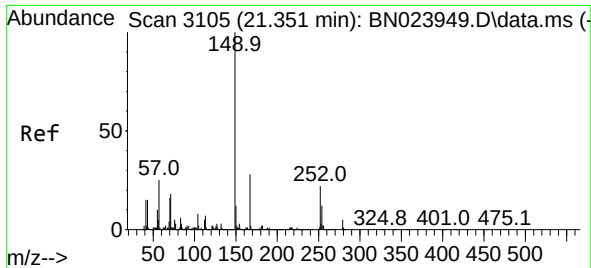

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2683.146 ng/ul m
 RT: 21.380 min Scan# 31
 Delta R.T. 0.030 min
 Lab File: BN023956.D
 Acq: 06 Feb 2023 17:11

Instrument :
 BNA_N
 ClientSampleId :
 A4488ME

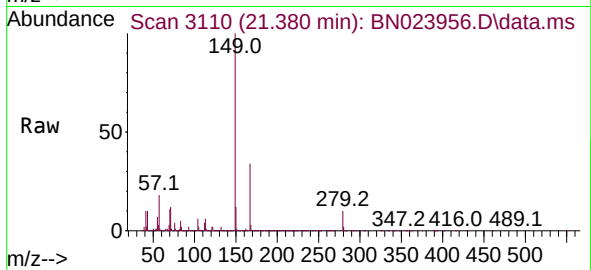

Tgt Ion:149 Resp:42951136
 Ion Ratio Lower Upper
 149 100
 167 34.5 22.7 34.1
 279 9.6 3.9 5.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2023
 Supervised By :mohammad ahmed 02/07/2023

