

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023959.D
 Acq On : 06 Feb 2023 19:02
 Operator : CG/JU
 Sample : 01362-05MEDL 20X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4443MEDL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2023
 Supervised By :mohammad ahmed 02/07/2023

Quant Time: Feb 07 03:01:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 07 02:28:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	132514	20.000	ng/u1	0.00
20) Naphthalene-d8	10.646	136	547124	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.493	164	349959	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.239	188	765205	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	649234	20.000	ng/u1	0.00
88) Perylene-d12	23.816	264	662626	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	3.693	84	7875m	0.866	ng/u1	0.04
7) Phenol-d5	7.011	99	13946	1.231	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	10694	1.496	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	11676	1.325	ng/u1	0.00
15) 4-Methylphenol-d8	8.558	113	10323	1.166	ng/u1	0.00
21) Nitrobenzene-d5	9.010	128	5412	1.239	ng/u1	0.00
24) 2-Nitrophenol-d4	9.728	143	4960	1.011	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	10465	1.145	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	16502	1.336	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	41580	1.537	ng/u1	0.00
49) Acenaphthylene-d8	14.187	160	36912	1.232	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.487	176	36746	1.613	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.339	188	49012	1.406	ng/u1	0.00
81) Pyrene-d10	19.633	212	58265	1.490	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.669	264	46763	1.379	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.345	149	708454	25.728	ng/u1	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023959.D
Acq On : 06 Feb 2023 19:02
Operator : CG/JU
Sample : 01362-05MEDL 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4443MEDL

Quant Time: Feb 07 03:01:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 07 02:28:26 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/07/2023
Supervised By :mohammad ahmed 02/07/2023

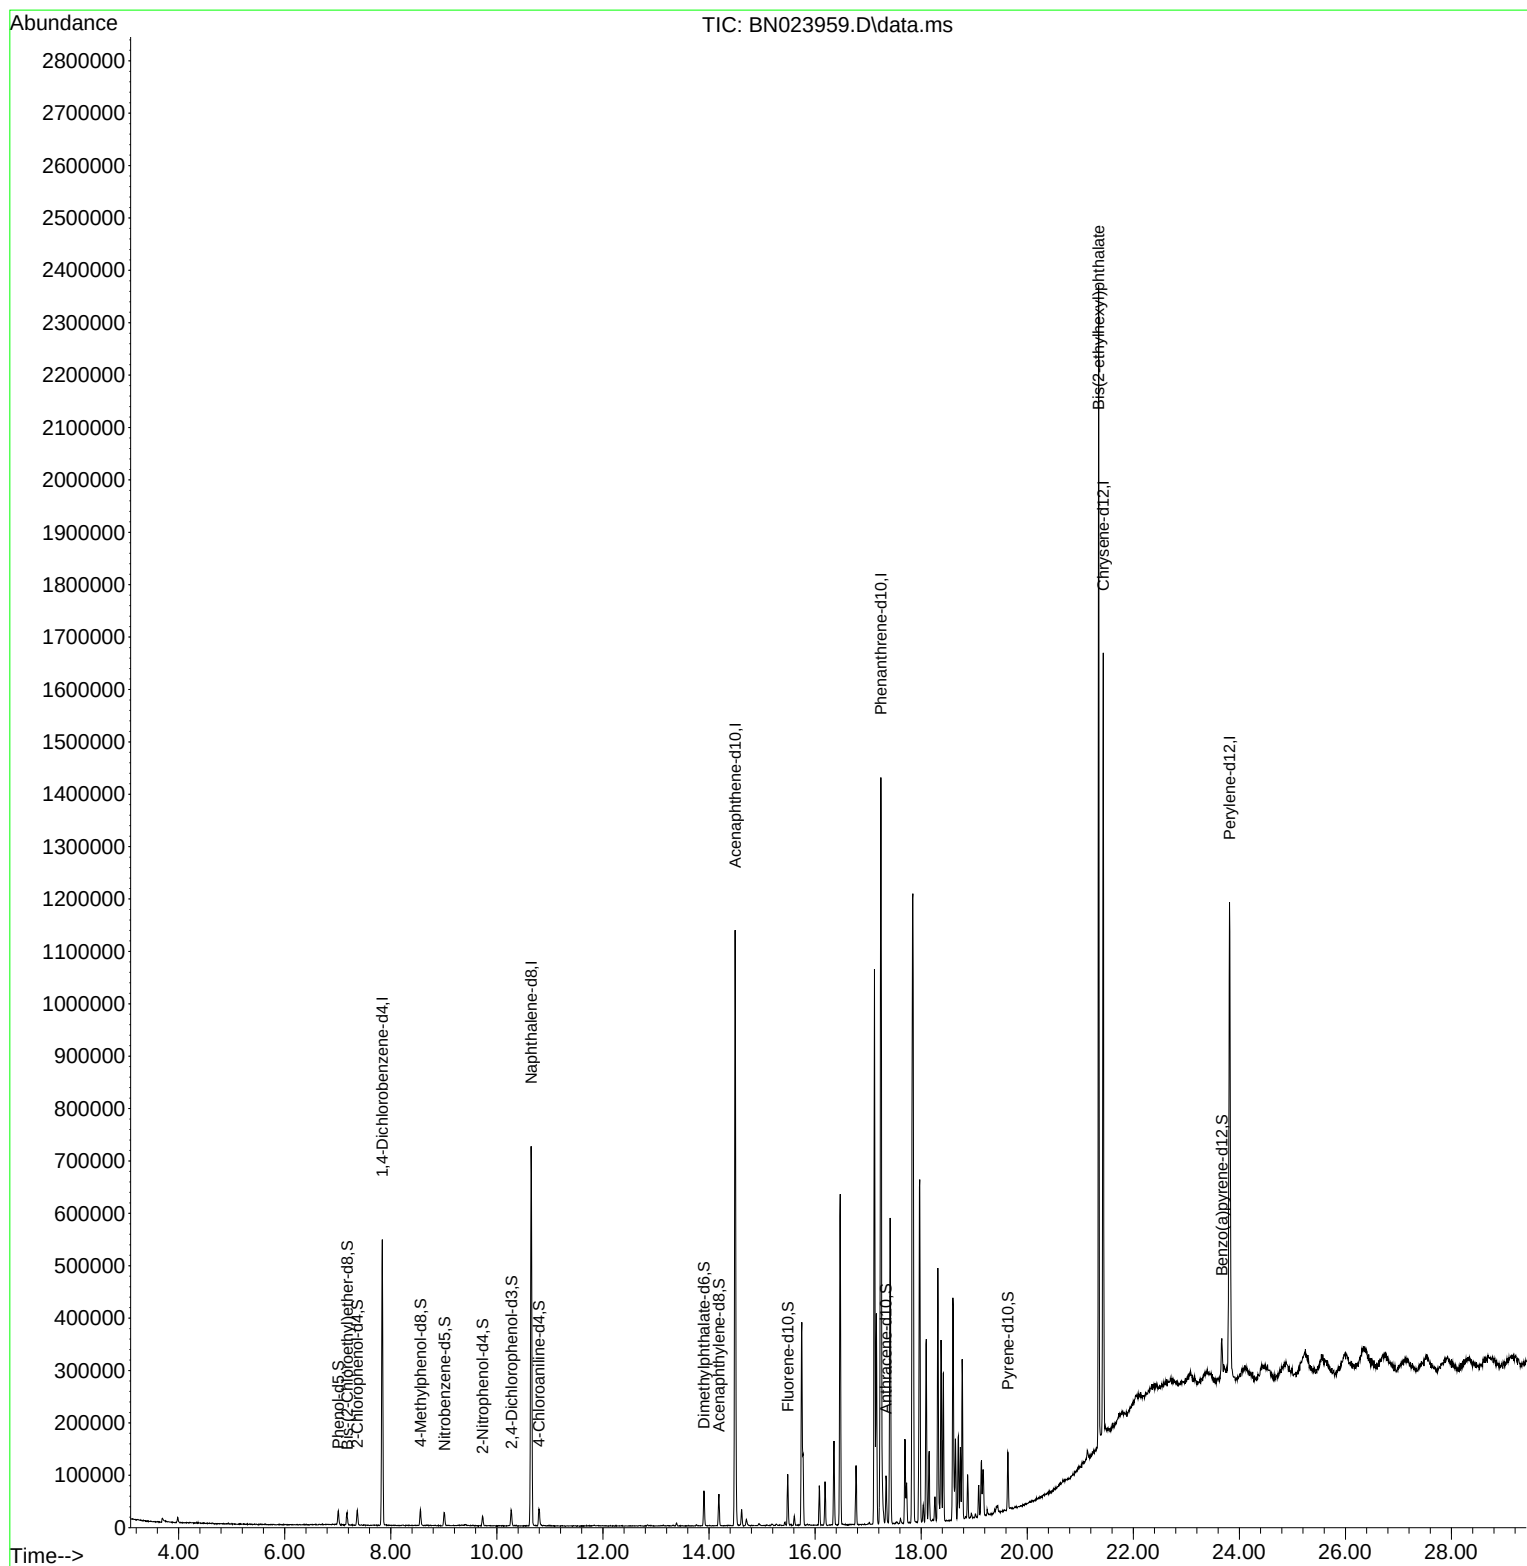

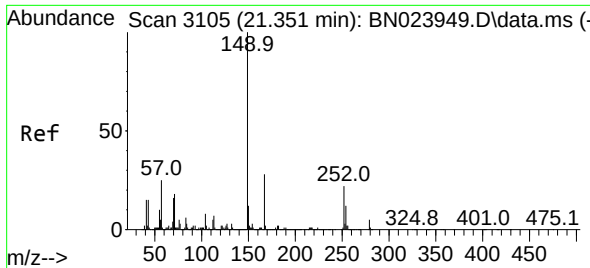

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 25.728 ng/ul
 RT: 21.345 min Scan# 3104
 Delta R.T. -0.006 min
 Lab File: BN023959.D
 Acq: 06 Feb 2023 19:02

Instrument :
 BNA_N
 ClientSampleId :
 A4443MEDL

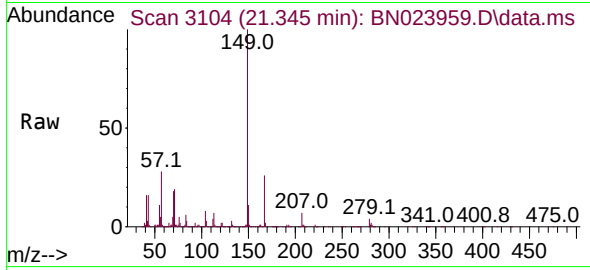

Tgt Ion:149 Resp: 708454
 Ion Ratio Lower Upper
 149 100
 167 26.2 22.7 34.1
 279 4.3 3.9 5.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/07/2023
 Supervised By :mohammad ahmed 02/07/2023

