

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023954.D
 Acq On : 06 Feb 2023 15:58
 Operator : CG/JU
 Sample : PB150667BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	30	rVB	39641	49590	1.74%	0.144%
2	3.652	93	96	115	rBV	465050	665150	23.31%	1.932%
3	3.981	149	152	159	rVB	11628	15653	0.55%	0.045%
4	4.969	315	320	321	rBV4	2442	2897	0.10%	0.008%
5	7.011	660	667	676	rVB	590530	890697	31.22%	2.587%
6	7.175	688	695	705	rVB	469327	723651	25.36%	2.102%
7	7.369	721	728	739	rVB	618208	941757	33.01%	2.735%
8	7.840	801	808	817	rVB	606373	919001	32.21%	2.669%
9	8.557	922	930	941	rBV	734683	1099859	38.55%	3.194%
10	9.010	999	1007	1017	rBV	557290	887815	31.12%	2.578%
11	9.728	1120	1129	1143	rBV	479953	776506	27.22%	2.255%
12	10.269	1214	1221	1231	rBV	734479	1158585	40.61%	3.365%
13	10.646	1278	1285	1293	rBV	777696	1293242	45.33%	3.756%
14	10.793	1303	1310	1326	rBV	730671	1184601	41.52%	3.440%
15	12.240	1548	1556	1564	rBV	12318	22497	0.79%	0.065%
16	13.122	1699	1706	1708	rBV6	2623	6065	0.21%	0.018%
17	13.769	1810	1816	1819	rBV5	3113	4387	0.15%	0.013%
18	13.910	1833	1840	1847	rBV	1293395	1709458	59.92%	4.964%
19	14.187	1880	1887	1899	rBV	1419521	1976531	69.28%	5.740%
20	14.492	1931	1939	1948	rBV	1271317	1765485	61.88%	5.127%
21	14.704	1968	1975	1991	rBV	578174	813875	28.53%	2.364%
22	14.940	2012	2015	2021	rVV	7697	10964	0.38%	0.032%
23	15.087	2039	2040	2045	rVB3	2453	3367	0.12%	0.010%
24	15.187	2054	2057	2064	rVB3	7686	11517	0.40%	0.033%
25	15.275	2066	2072	2077	rBV7	3884	7559	0.26%	0.022%
26	15.487	2100	2108	2119	rBV	1827192	2477431	86.84%	7.195%
27	15.610	2123	2129	2140	rVV	582834	738067	25.87%	2.143%
28	15.722	2144	2148	2154	rVV2	7122	11513	0.40%	0.033%
29	16.057	2202	2205	2208	rBV5	2675	3119	0.11%	0.009%
30	16.275	2238	2242	2246	rBV7	2437	3990	0.14%	0.012%
31	17.245	2400	2407	2417	rBV	1460838	2029090	71.12%	5.893%
32	17.339	2417	2423	2435	rVV	1833977	2557072	89.63%	7.426%
33	17.863	2509	2512	2519	rVB	8056	11193	0.39%	0.033%
34	18.139	2556	2559	2567	rBV3	19872	31099	1.09%	0.090%
35	18.216	2568	2572	2580	rVB	17012	23707	0.83%	0.069%
36	18.992	2701	2704	2705	rBV3	3413	3976	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
 Data File : BN023954.D
 Acq On : 06 Feb 2023 15:58
 Operator : CG/JU
 Sample : PB150667BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Title : SVOA CALIBRATION

37	19.204	2736	2740	2746	rVB2	23336	30541	1.07%	0.089%
38	19.269	2748	2751	2755	rBV	18538	27845	0.98%	0.081%
39	19.422	2775	2777	2780	rBV3	12171	12522	0.44%	0.036%
40	19.639	2808	2814	2824	rBV	2207849	2853022	100.00%	8.285%
41	21.439	3115	3120	3125	rBV	1568298	1950378	68.36%	5.664%
42	23.668	3492	3499	3513	rVB	1387735	2786859	97.68%	8.093%
43	23.816	3518	3524	3532	rVB2	985496	1941887	68.06%	5.639%


Sum of corrected areas: 34434020

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023954.D
Acq On : 06 Feb 2023 15:58
Operator : CG/JU
Sample : PB150667BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

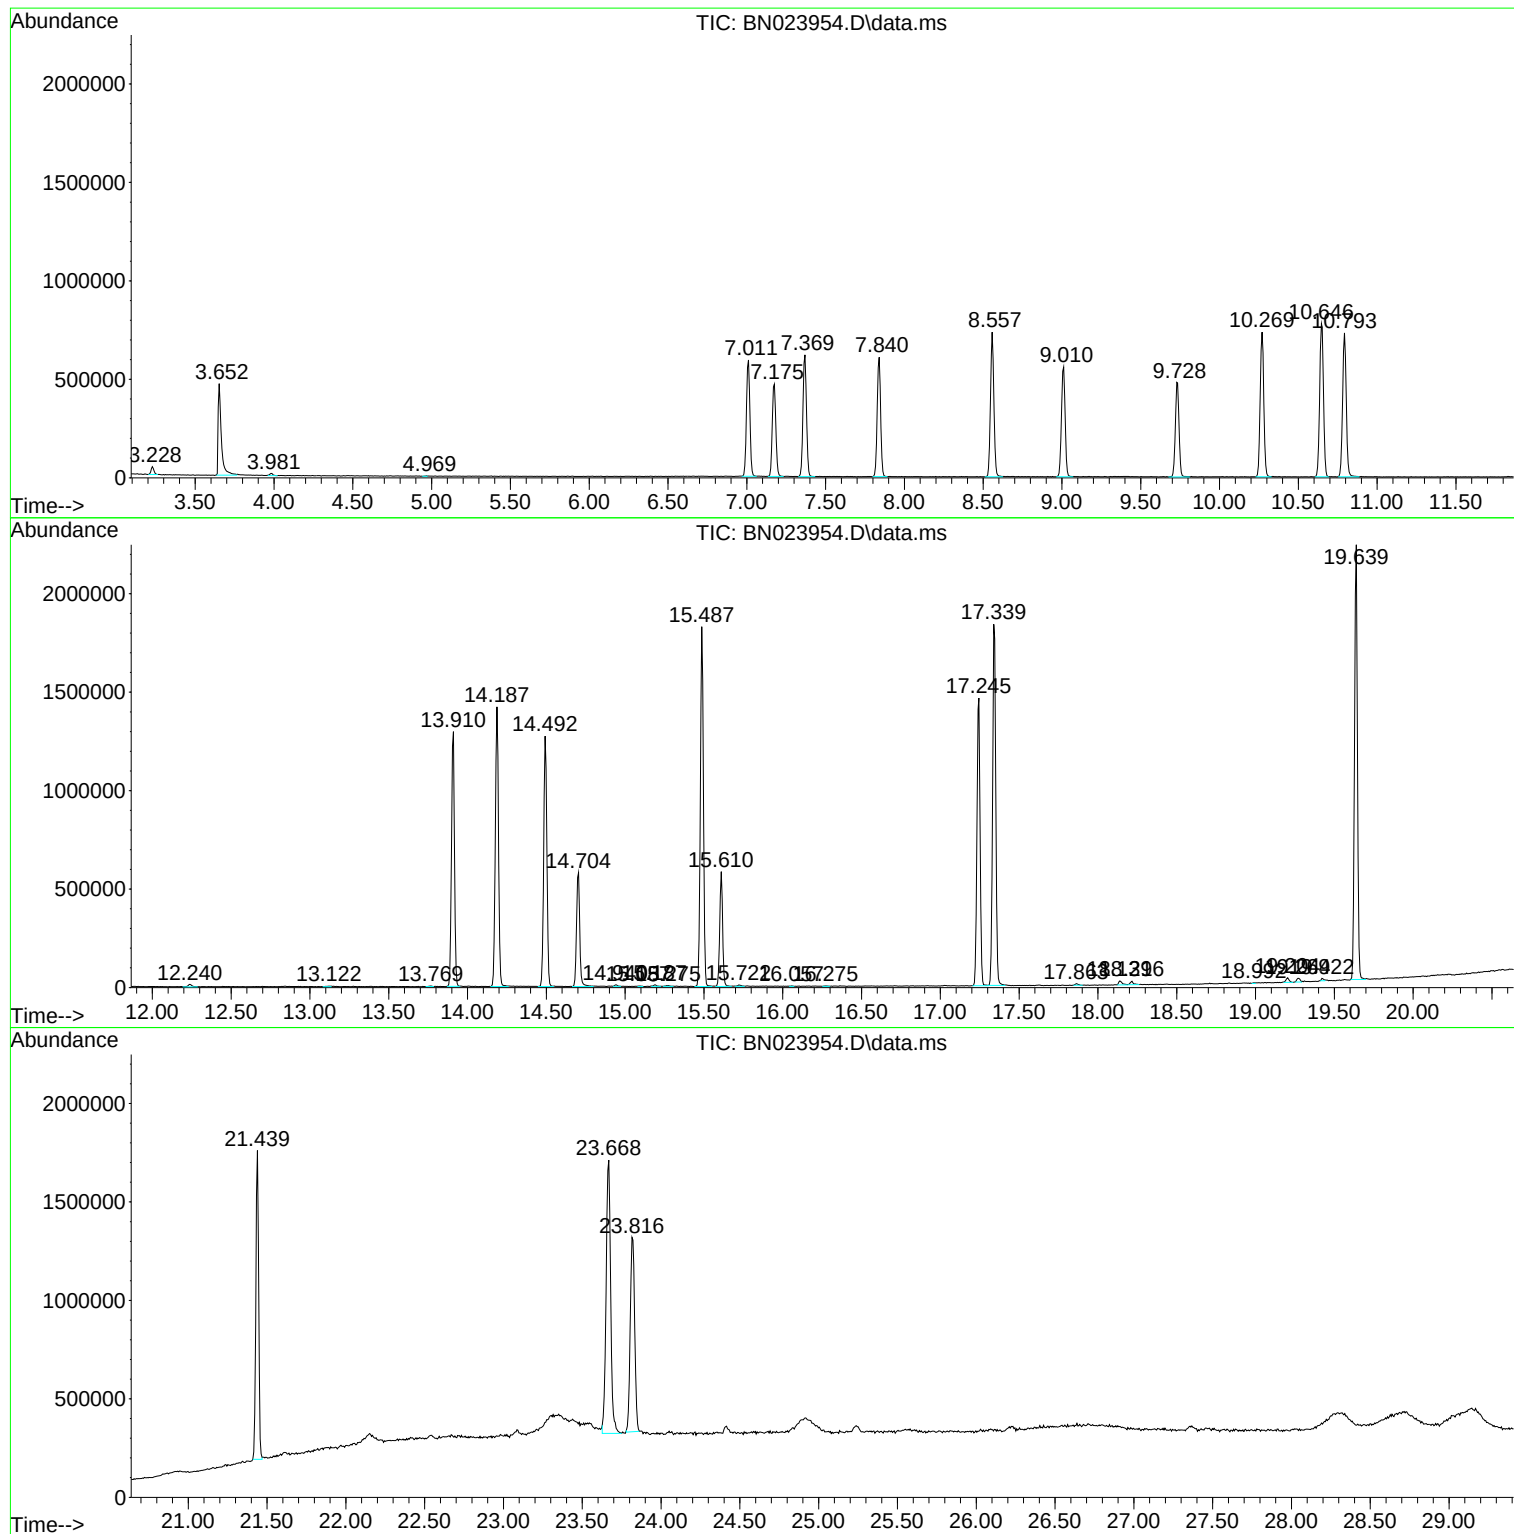

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023954.D
Acq On : 06 Feb 2023 15:58
Operator : CG/JU
Sample : PB150667BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020623\
Data File : BN023954.D
Acq On : 06 Feb 2023 15:58
Operator : CG/JU
Sample : PB150667BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc