
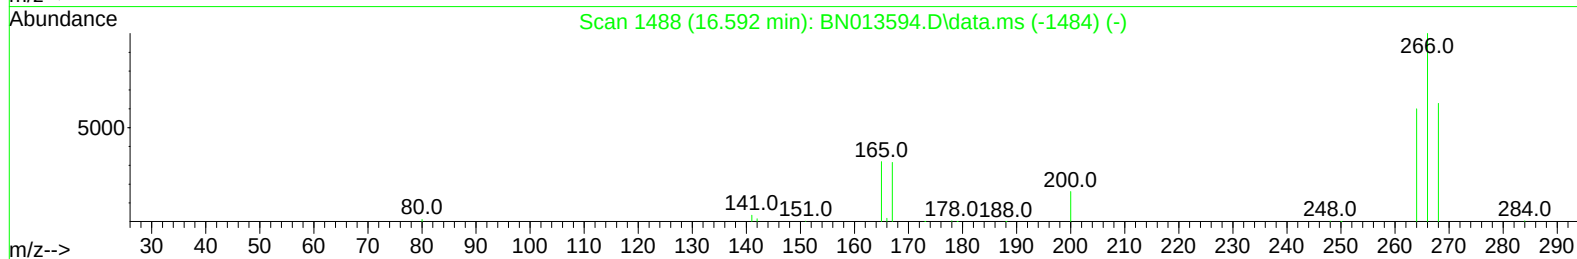
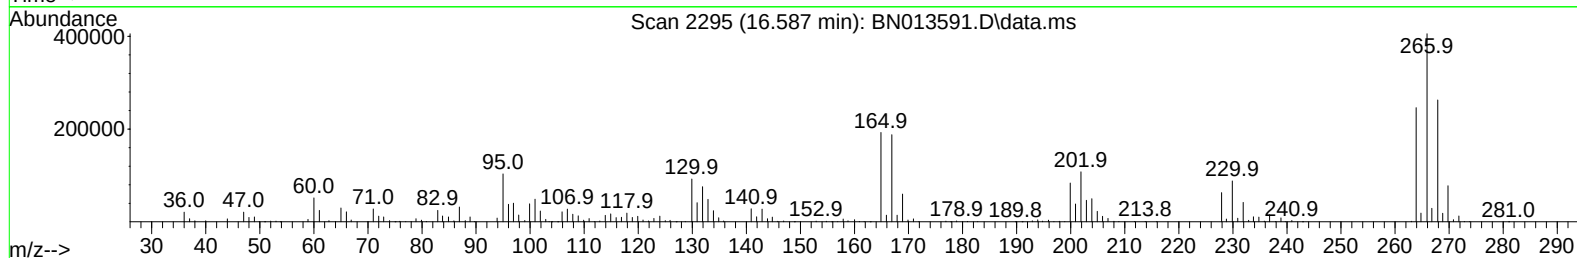


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020821\
 Data File : BN013591.D
 Acq On : 08 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 16:58:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 08 15:13:18 2021
 Response via : Initial Calibration

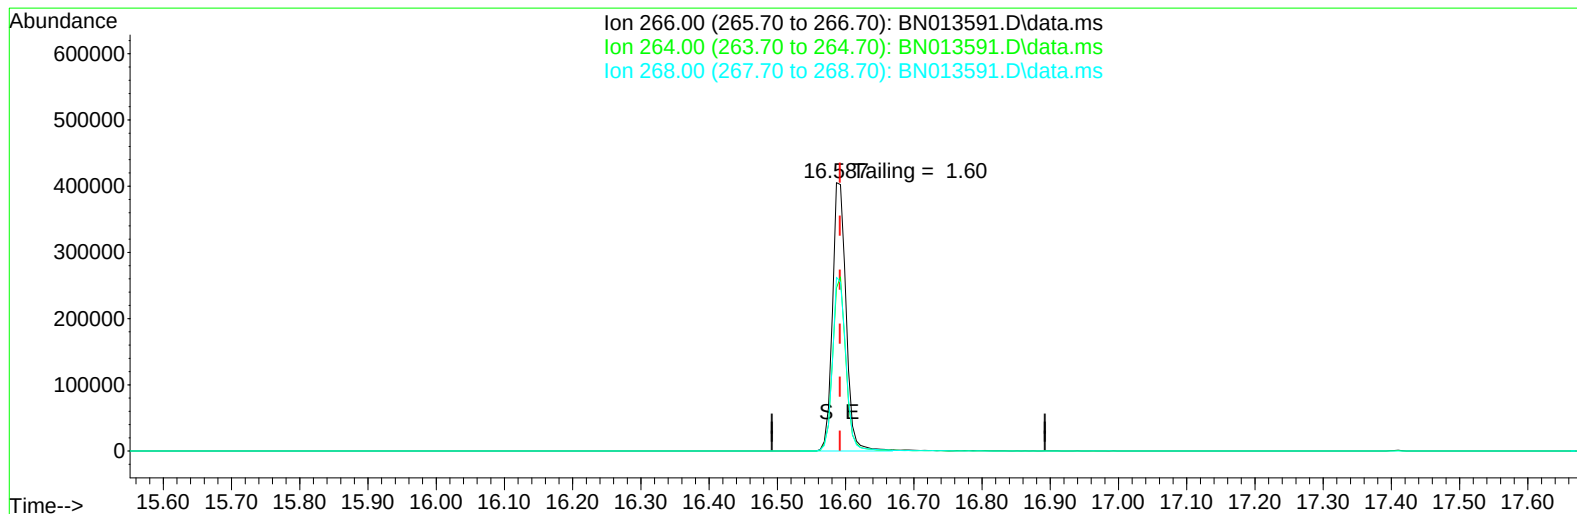

TIC: BN013591.D\data.ms

(24) Pentachlorophenol

16.587min (-0.005) 0.00 ng

response 562853

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.14
268.00	68.30	63.95
0.00	0.00	0.00