

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020821\
 Data File : BN013596.D
 Acq On : 08 Feb 2021 13:12
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Feb 08 13:41:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 08 12:46:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.555	152	6196	0.40	ng	0.00
7) Naphthalene-d8	10.315	136	23501	0.40	ng	# 0.00
13) Acenaphthene-d10	14.181	164	13162	0.40	ng	0.00
19) Phenanthrene-d10	16.933	188	27228	0.40	ng	# 0.00
29) Chrysene-d12	21.141	240	27996	0.40	ng	# 0.00
36) Perylene-d12	23.305	264	22788	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.180	112	20978	1.16	ng	0.00
5) Phenol-d6	6.734	99	26476	1.15	ng	0.00
8) Nitrobenzene-d5	8.693	82	21218	1.34	ng	0.00
11) 2-Methylnaphthalene-d10	11.911	152	60887	1.45	ng	0.00
14) 2,4,6-Tribromophenol	15.678	330	6216	1.09	ng	0.00
15) 2-Fluorobiphenyl	12.798	172	79770	1.38	ng	0.00
27) Fluoranthene-d10	18.977	212	121568	1.41	ng	0.00
31) Terphenyl-d14	19.588	244	99312	1.38	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.182	88	10754	1.40	ng	98
3) n-Nitrosodimethylamine	3.488	42	8681	1.29	ng	98
6) bis(2-Chloroethyl)ether	6.992	93	24768	1.37	ng	99
9) Naphthalene	10.365	128	95131	1.35	ng	99
10) Hexachlorobutadiene	10.657	225	15728	1.27	ng	# 100
12) 2-Methylnaphthalene	11.982	142	66044	1.36	ng	99
16) Acenaphthylene	13.902	152	84589	1.35	ng	100
17) Acenaphthene	14.245	154	60988	1.35	ng	99
18) Fluorene	15.234	166	75358	1.32	ng	100
20) 4,6-Dinitro-2-methylph...	15.323	198	5116	1.53	ng	# 53
21) 4-Bromophenyl-phenylether	16.142	248	22528	1.33	ng	# 75
22) Hexachlorobenzene	16.252	284	24531	1.30	ng	99
23) Atrazine	16.410	200	14057	1.30	ng	95
24) Pentachlorophenol	16.592	266	5645	1.00	ng	97
25) Phenanthrene	16.970	178	121515	1.33	ng	100
26) Anthracene	17.067	178	102142	1.32	ng	100
28) Fluoranthene	19.002	202	139043	1.34	ng	99
30) Pyrene	19.369	202	135739	1.32	ng	100
32) Benzo(a)anthracene	21.120	228	122537	1.25	ng	98
33) Chrysene	21.173	228	138225	1.27	ng	98
34) Bis(2-ethylhexyl)phtha...	21.077	149	32480	1.07	ng	100
35) Indeno(1,2,3-cd)pyrene	25.451	276	145774	1.28	ng	98
37) Benzo(b)fluoranthene	22.662	252	132911	1.41	ng	# 92
38) Benzo(k)fluoranthene	22.703	252	139203	1.52	ng	# 91
39) Benzo(a)pyrene	23.209	252	113481	1.46	ng	# 89
40) Dibenzo(a,h)anthracene	25.468	278	125201	1.44	ng	96
41) Benzo(g,h,i)perylene	26.105	276	127960	1.44	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020821\
Data File : BN013596.D
Acq On : 08 Feb 2021 13:12
Operator : CG/JU
Sample : SSTDIC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC1.6

Quant Time: Feb 08 13:41:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 08 12:46:36 2021
Response via : Initial Calibration




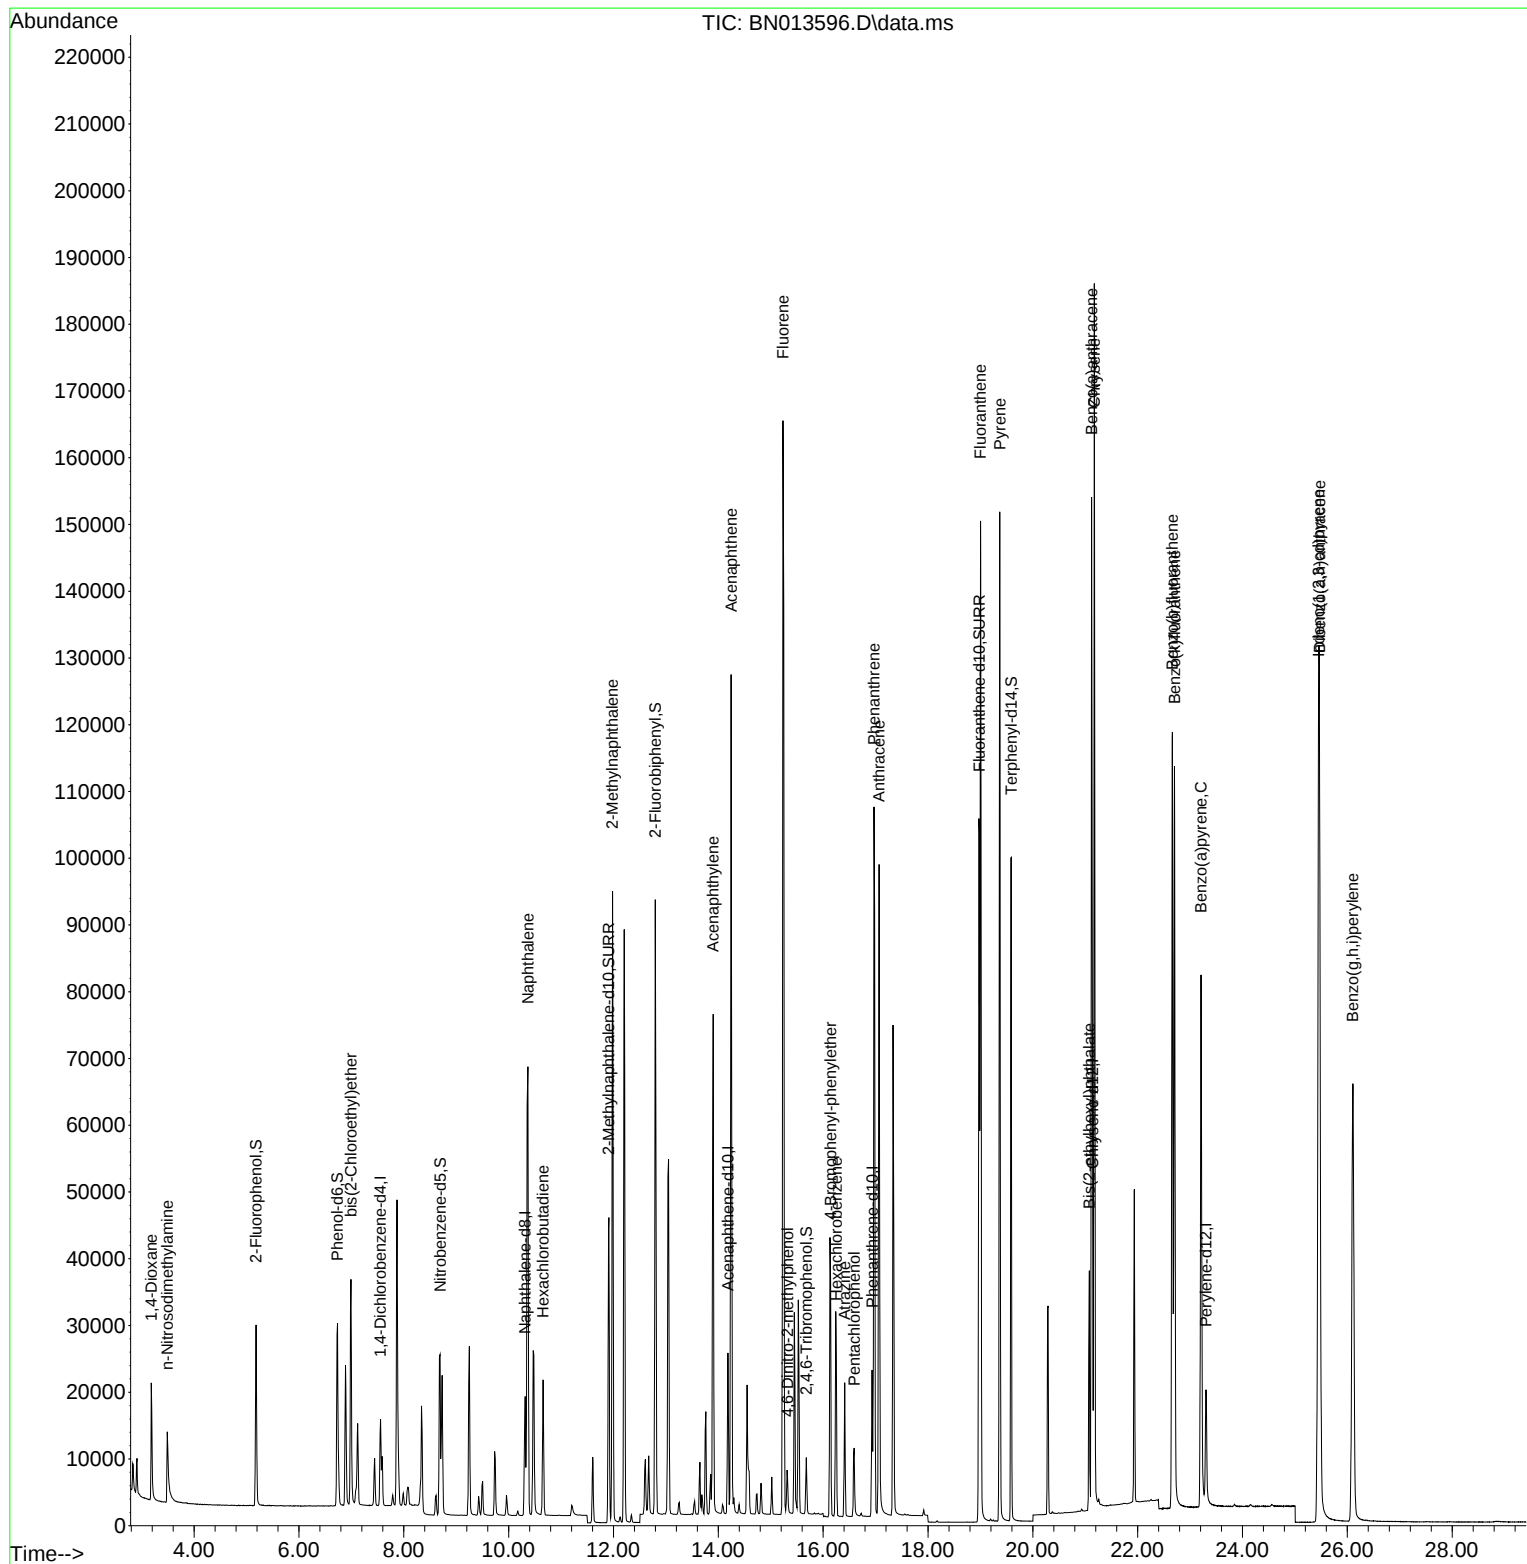




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.555 min Scan# 593
 Delta R.T. 0.000 min
 Lab File: BN013596.D
 Acq: 08 Feb 2021 13:12




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:152 Resp: 6196
 Ion Ratio Lower Upper
 152 100
 150 154.8 121.8 182.8
 115 58.1 46.6 69.8

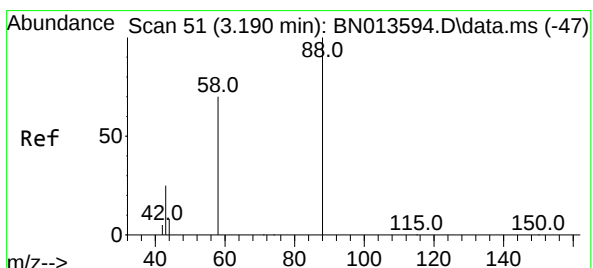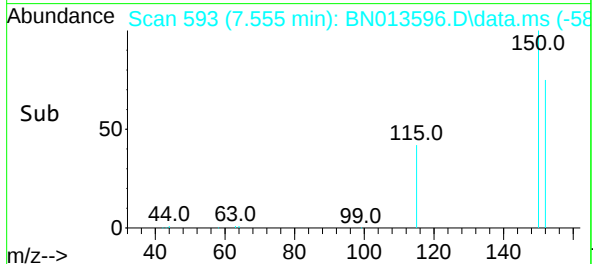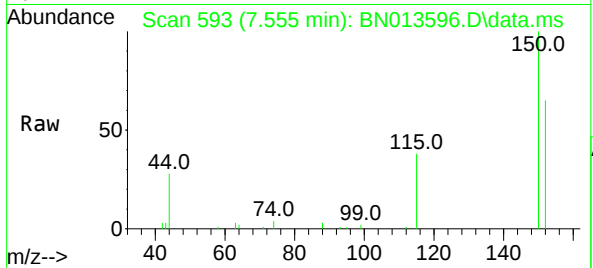

#2
 1,4-Dioxane
 Concen: 1.40 ng
 RT: 3.182 min Scan# 50
 Delta R.T. -0.008 min
 Lab File: BN013596.D
 Acq: 08 Feb 2021 13:12

Tgt Ion: 88 Resp: 10754
 Ion Ratio Lower Upper
 88 100
 58 79.9 64.6 96.8
 43 30.2 26.6 40.0

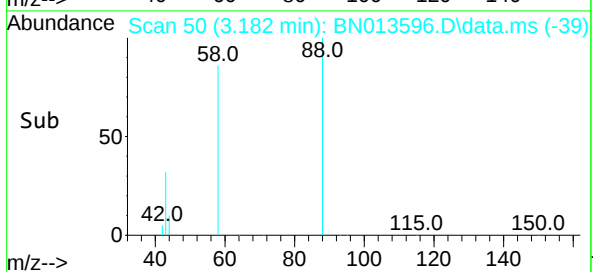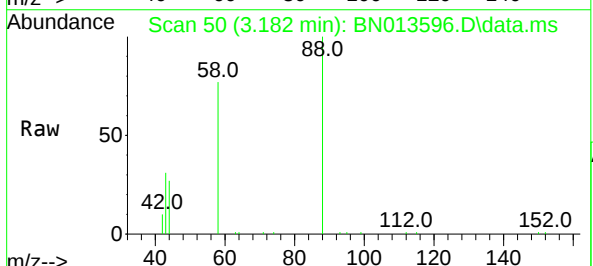







#3
n-Nitrosodimethylamine
Concen: 1.29 ng
RT: 3.488 min Scan# 88
Delta R.T. -0.008 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion: 42 Resp: 8681




Ion	Ratio	Lower	Upper
42	100		
74	121.5	95.0	142.6
44	7.3	5.8	8.8

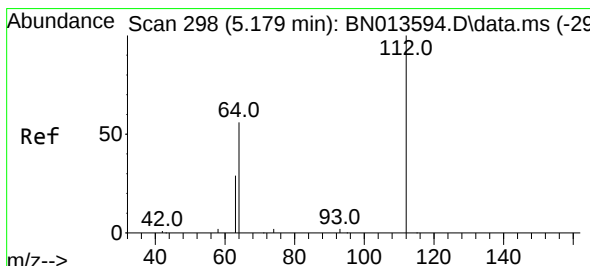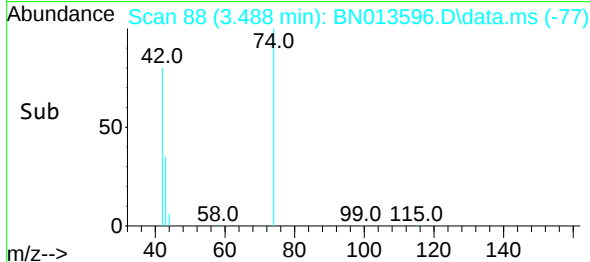


#4
2-Fluorophenol
Concen: 1.16 ng
RT: 5.180 min Scan# 298
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion: 112 Resp: 20978

Ion	Ratio	Lower	Upper
112	100		
64	55.7	44.3	66.5
63	28.6	23.0	34.6


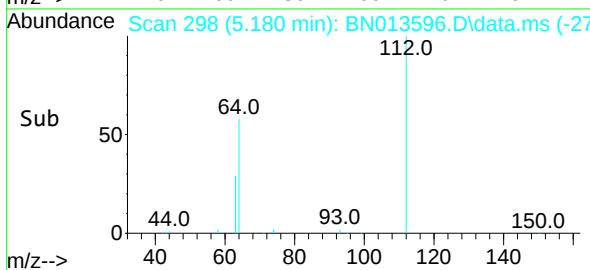

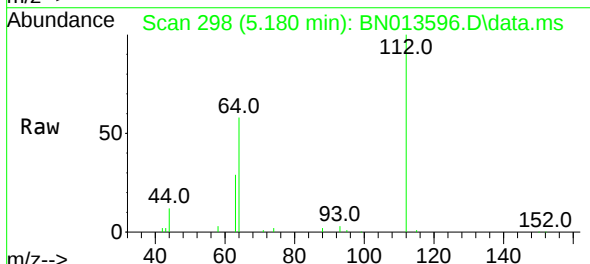




#5
Phenol-d6
Concen: 1.15 ng
RT: 6.734 min Scan# 491
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	99	Resp:	26476
Ion	Ratio	Lower	Upper
99	100		
42	19.0	15.2	22.8
71	31.3	26.1	39.1

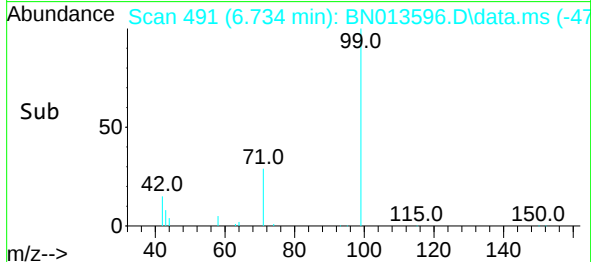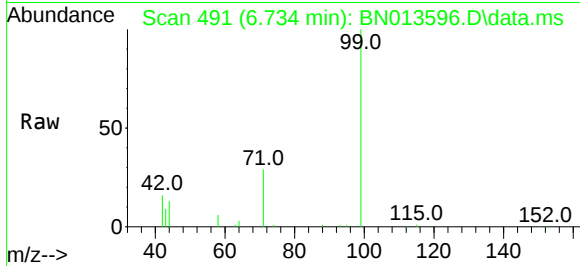

#6
bis(2-Chloroethyl)ether
Concen: 1.37 ng
RT: 6.992 min Scan# 523
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12


Tgt Ion:	93	Resp:	24768
Ion	Ratio	Lower	Upper
93	100		
63	77.2	60.8	91.2
95	32.9	26.0	39.0

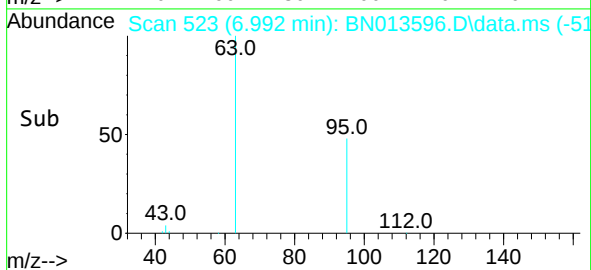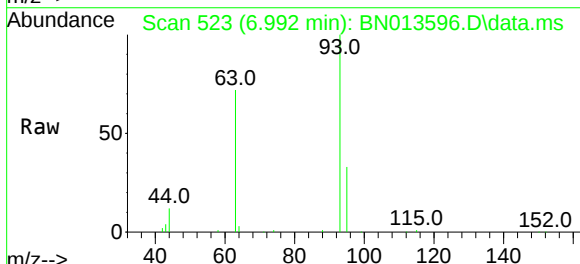





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.315 min Scan# 845
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6







Tgt Ion:	136	Resp:	23501
Ion Ratio	Lower	Upper	
136	100		
137	11.1	9.0	13.6
54	5.9	6.4	9.6#
68	4.4	4.5	6.7#



#8
Nitrobenzene-d5
Concen: 1.34 ng
RT: 8.693 min Scan# 717
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:	82	Resp:	21218
Ion Ratio	Lower	Upper	
82	100		
128	50.7	39.2	58.8
54	45.7	40.1	60.1


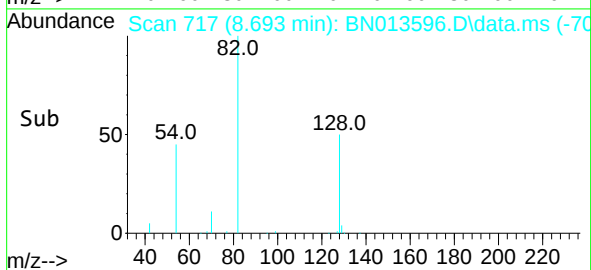

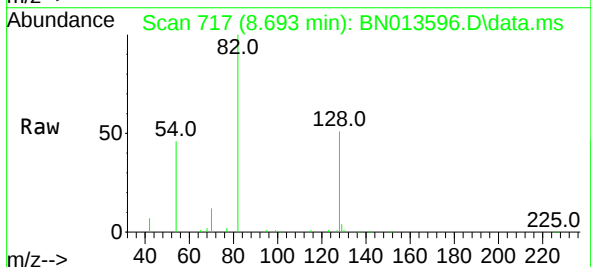


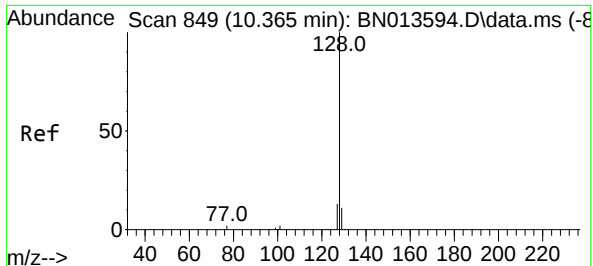

#9
Naphthalene
Concen: 1.35 ng
RT: 10.365 min Scan# 849
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	128	Resp:	95131
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.0	13.4
127	12.7	10.4	15.6

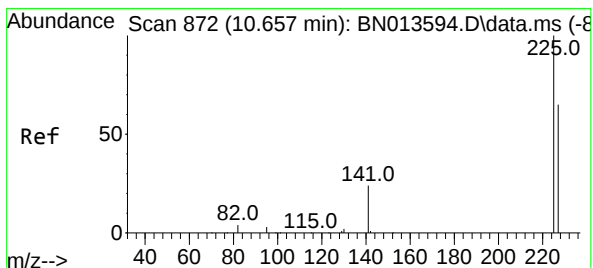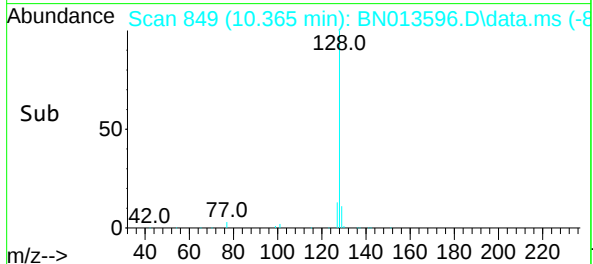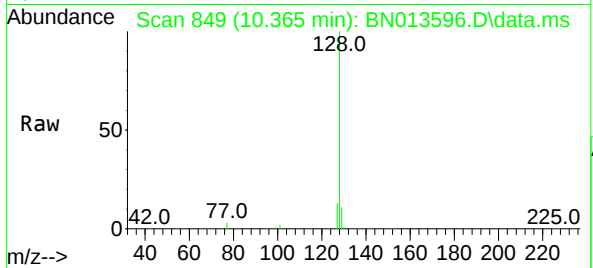

#10
Hexachlorobutadiene
Concen: 1.27 ng
RT: 10.657 min Scan# 872
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:	225	Resp:	15728
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.1	51.2	76.8


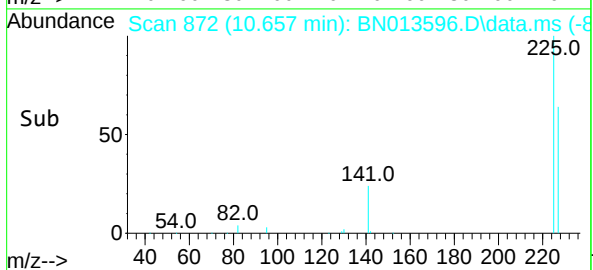

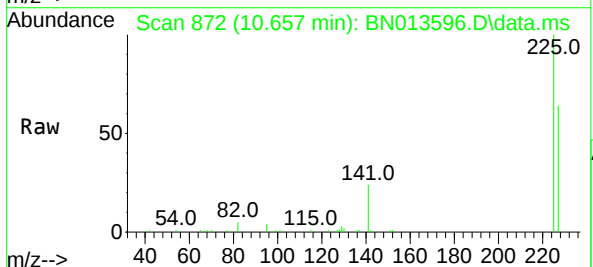


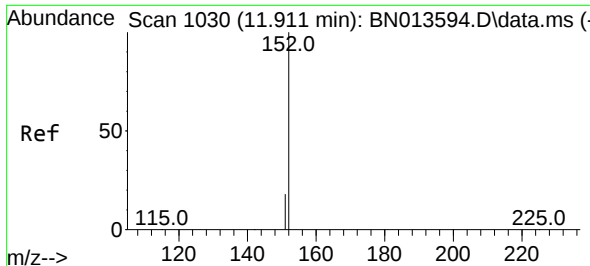

#11
2-Methylnaphthalene-d10
Concen: 1.45 ng
RT: 11.911 min Scan# 1030
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 60887
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.2

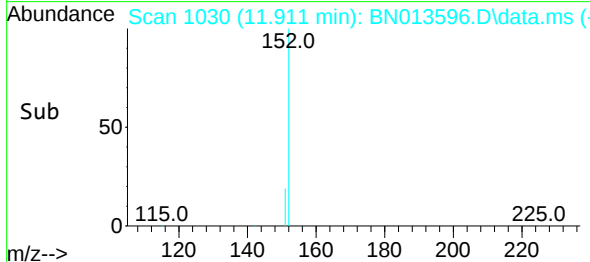

#12
2-Methylnaphthalene
Concen: 1.36 ng
RT: 11.982 min Scan# 1046
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:142 Resp: 66044
Ion Ratio Lower Upper
142 100
141 88.1 70.5 105.7
115 32.2 27.4 41.0


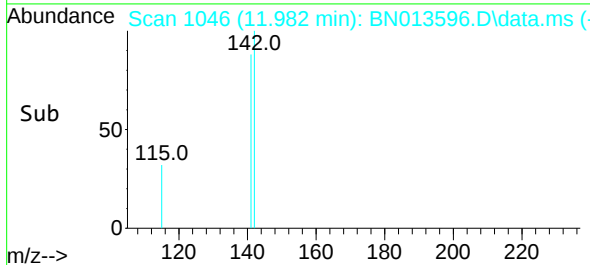

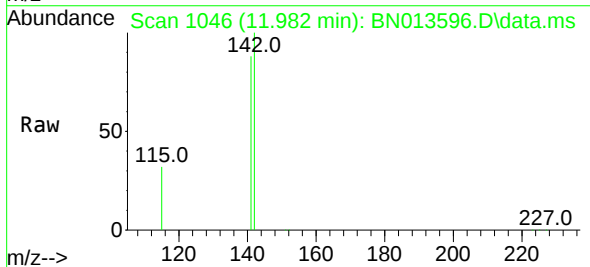




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.181 min Scan# 1296
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 13162
Ion Ratio Lower Upper
164 100
162 102.8 79.6 119.4
160 46.2 36.0 54.0

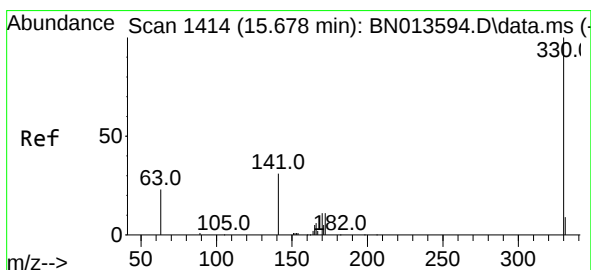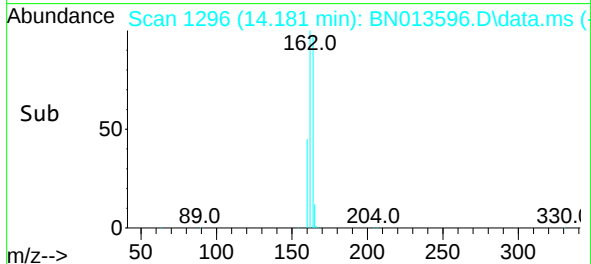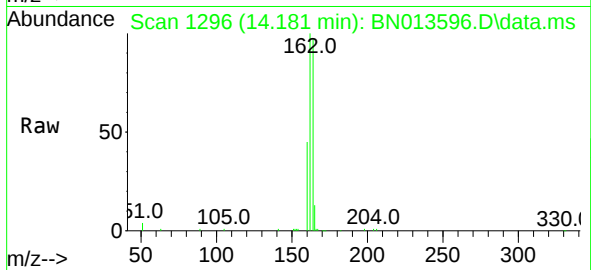

#14
2,4,6-Tribromophenol
Concen: 1.09 ng
RT: 15.678 min Scan# 1414
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:330 Resp: 6216
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.3 26.8 40.2


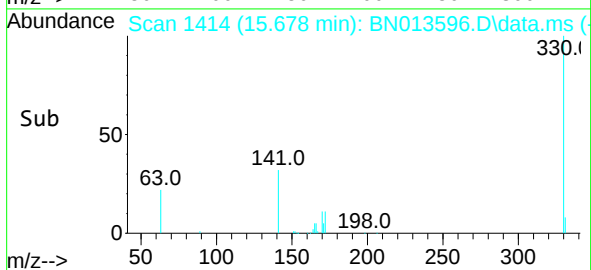

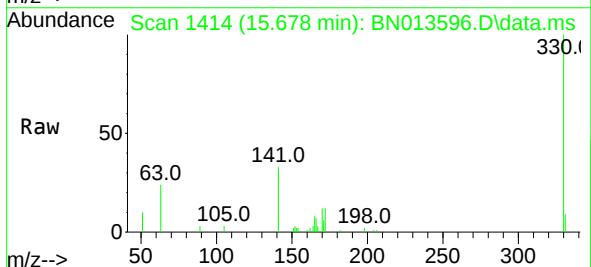


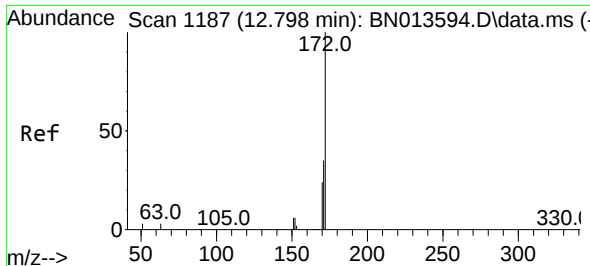

#15
2-Fluorobiphenyl
Concen: 1.38 ng
RT: 12.798 min Scan# 1187
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172	Resp:	79770
Ion	Ratio	Lower Upper
172	100	
171	35.4	28.6 42.8
170	23.5	18.9 28.3

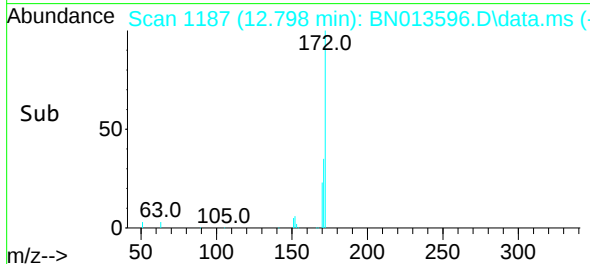

#16
Acenaphthylene
Concen: 1.35 ng
RT: 13.902 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:152	Resp:	84589
Ion	Ratio	Lower Upper
152	100	
151	19.4	15.7 23.5
153	13.0	10.5 15.7


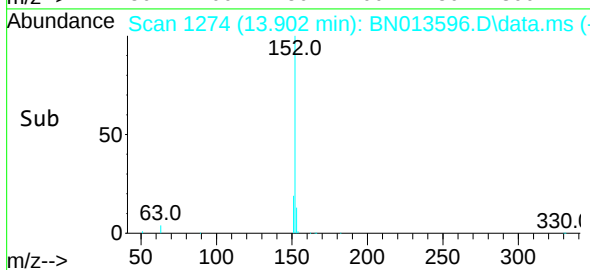

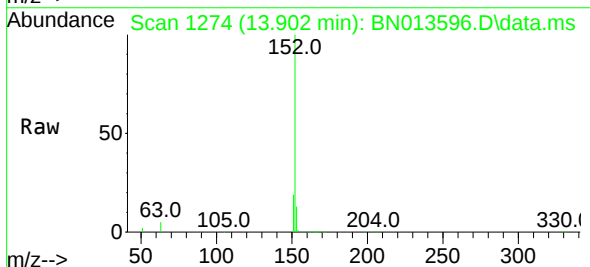




#17
Acenaphthene
Concen: 1.35 ng
RT: 14.245 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 60988
Ion Ratio Lower Upper
154 100
153 110.1 88.4 132.6
152 53.0 43.0 64.4

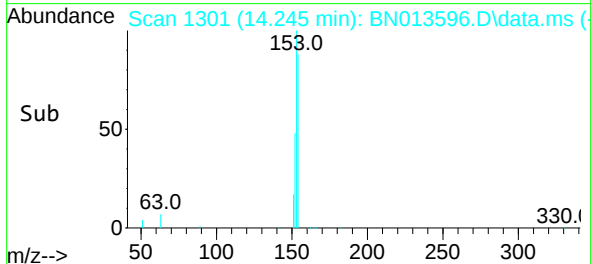

#18
Fluorene
Concen: 1.32 ng
RT: 15.234 min Scan# 1379
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:166 Resp: 75358
Ion Ratio Lower Upper
166 100
165 97.1 77.8 116.8
167 13.4 10.6 16.0


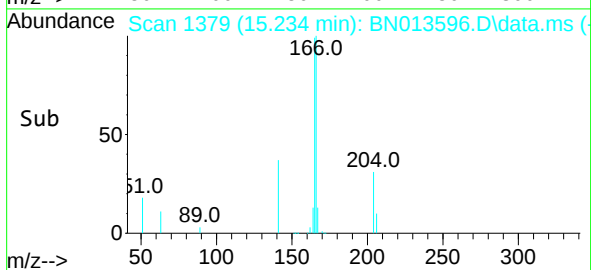

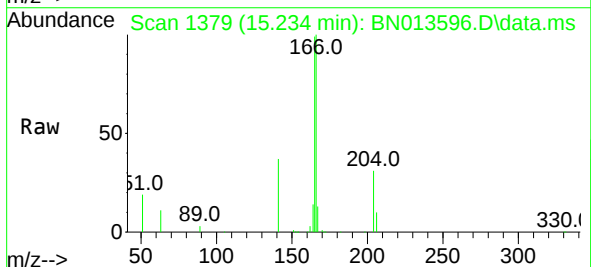


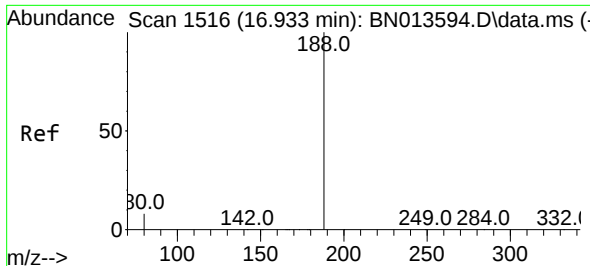

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.933 min Scan# 1516
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 27228
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.7 9.0 13.6#

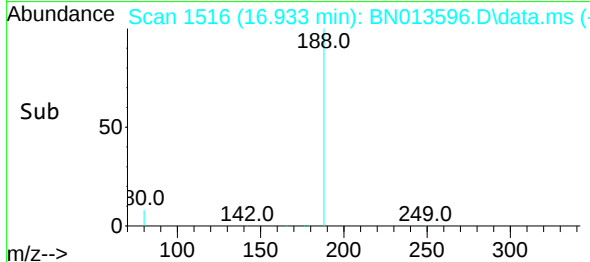

#20
4,6-Dinitro-2-methylphenol
Concen: 1.53 ng
RT: 15.323 min Scan# 1386
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:198 Resp: 5116
Ion Ratio Lower Upper
198 100
51 28.8 61.7 92.5#
105 21.9 33.0 49.6#


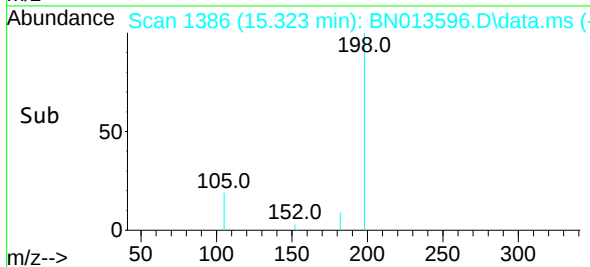

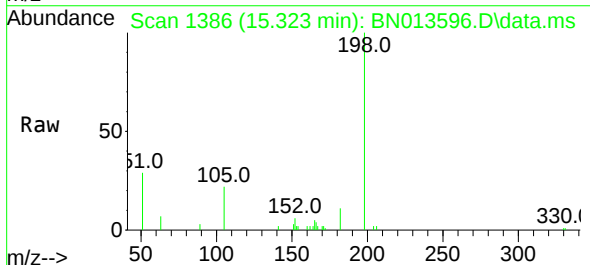


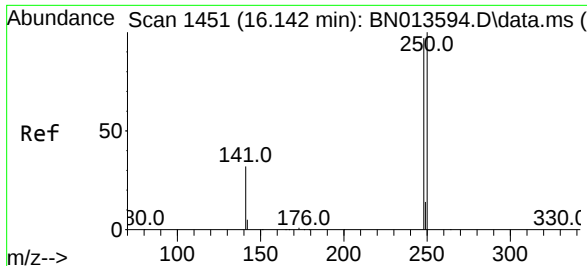

#21
4-Bromophenyl-phenylether
Concen: 1.33 ng
RT: 16.142 min Scan# 1451
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 22528
Ion Ratio Lower Upper
248 100
250 104.9 75.5 113.3
141 30.9 53.8 80.8#

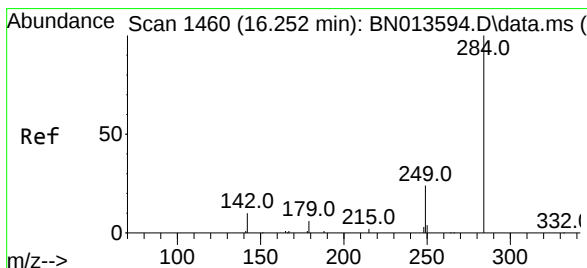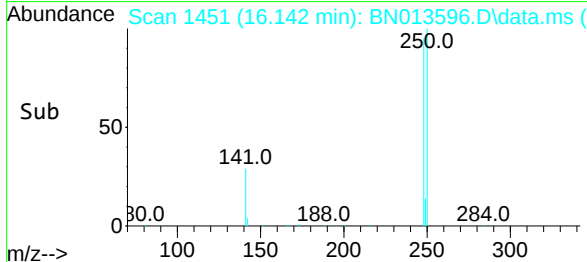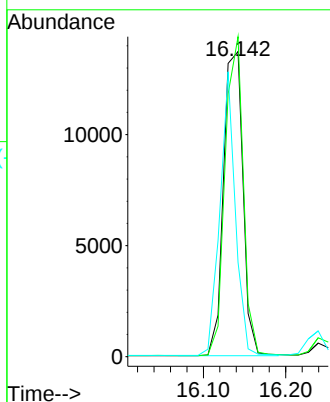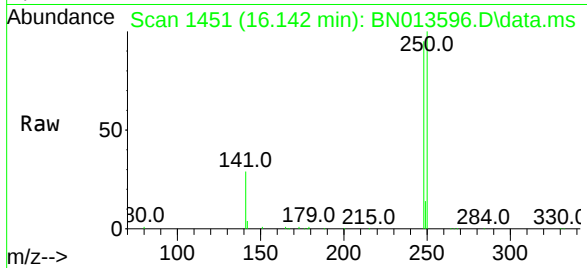

#22
Hexachlorobenzene
Concen: 1.30 ng
RT: 16.252 min Scan# 1460
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:284 Resp: 24531
Ion Ratio Lower Upper
284 100
142 35.5 27.9 41.9
249 30.6 24.2 36.2


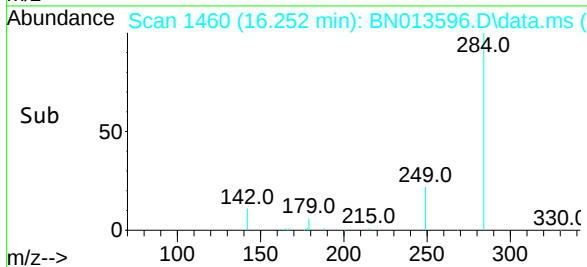
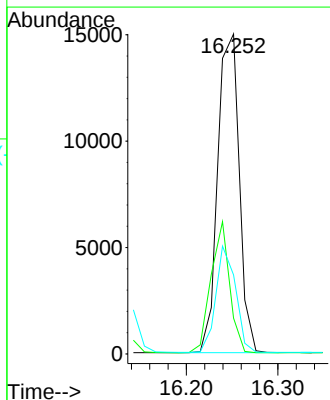
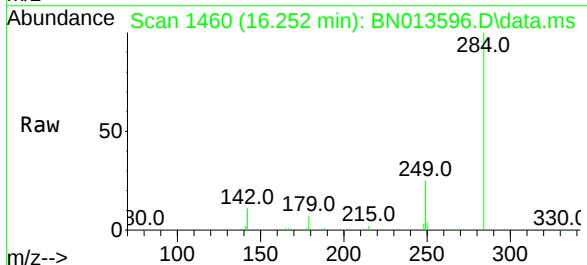


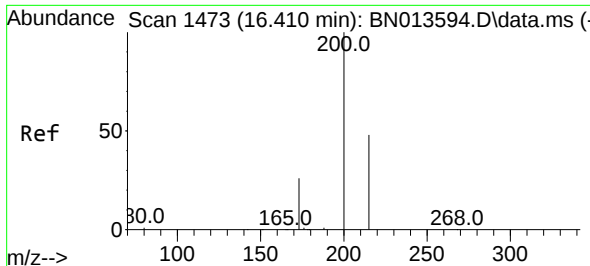

#23
Atrazine
Concen: 1.30 ng
RT: 16.410 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 14057
Ion Ratio Lower Upper
200 100
173 26.3 18.6 28.0
215 48.1 41.0 61.6

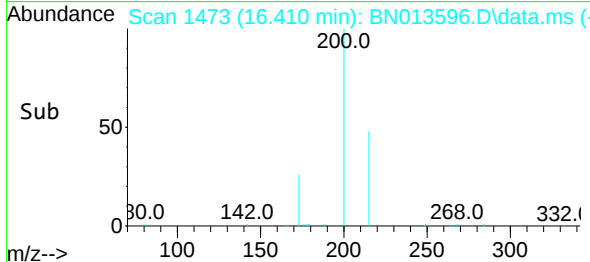

#24
Pentachlorophenol
Concen: 1.00 ng
RT: 16.592 min Scan# 1488
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:266 Resp: 5645
Ion Ratio Lower Upper
266 100
264 63.5 51.6 77.4
268 65.0 54.6 82.0


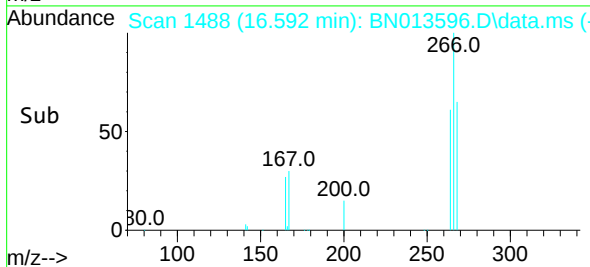

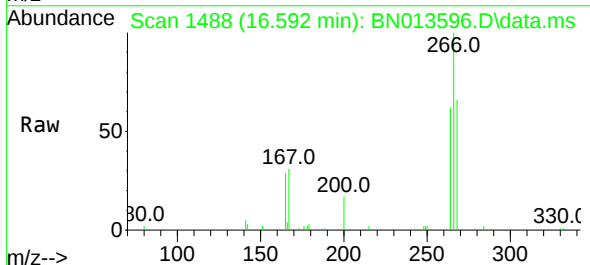




#25
Phenanthrene
Concen: 1.33 ng
RT: 16.970 min Scan# 1519
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 121515
Ion Ratio Lower Upper
178 100
176 18.5 15.0 22.4
179 15.2 12.3 18.5

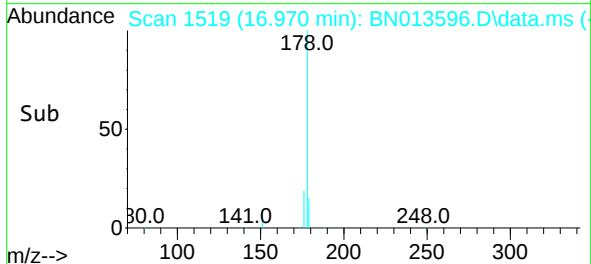

#26
Anthracene
Concen: 1.32 ng
RT: 17.067 min Scan# 1527
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:178 Resp: 102142
Ion Ratio Lower Upper
178 100
176 18.0 14.6 21.8
179 15.2 12.2 18.2


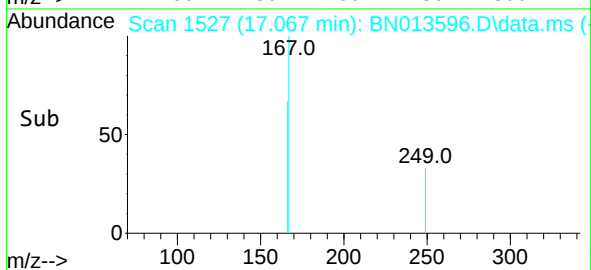

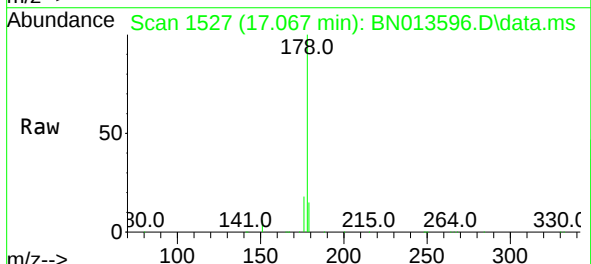


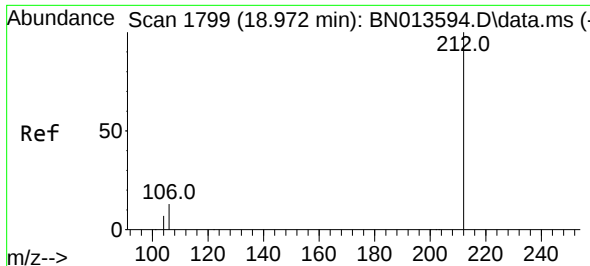

#27
Fluoranthene-d10
Concen: 1.41 ng
RT: 18.977 min Scan# 1800
Delta R.T. 0.005 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 121568
Ion Ratio Lower Upper
212 100
106 12.9 9.7 14.5
104 7.2 5.5 8.3

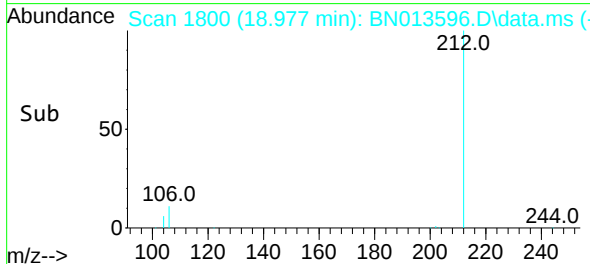

#28
Fluoranthene
Concen: 1.34 ng
RT: 19.002 min Scan# 1805
Delta R.T. -0.005 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:202 Resp: 139043
Ion Ratio Lower Upper
202 100
101 10.9 8.1 12.1
203 17.3 13.9 20.9

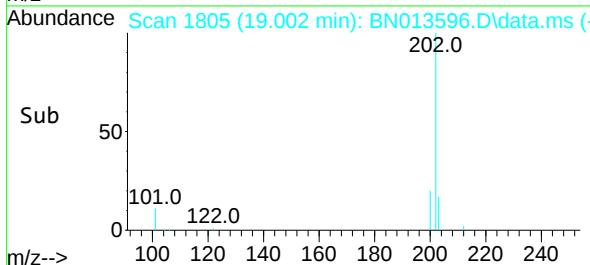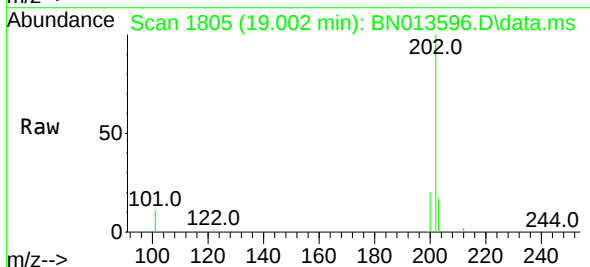



#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.141 min Scan# 2114

Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12





Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6

Tgt Ion:240	Resp:	27996
Ion Ratio	Lower	Upper
240	100	
120	6.2	10.2 15.4#
236	25.1	21.3 31.9

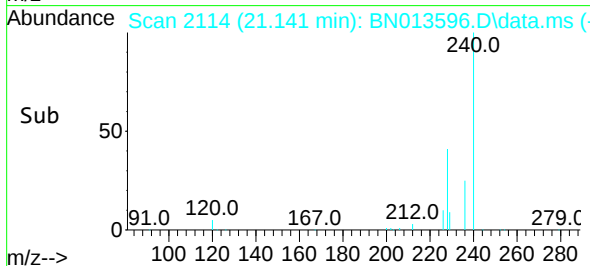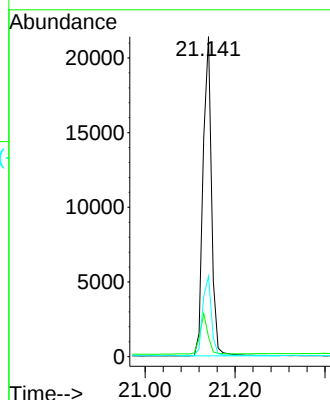

#30

Pyrene

Concen: 1.32 ng




RT: 19.369 min Scan# 1879


Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12

Tgt Ion:202	Resp:	135739
Ion Ratio	Lower	Upper
202	100	
200	20.2	16.3 24.5
203	17.4	14.0 21.0


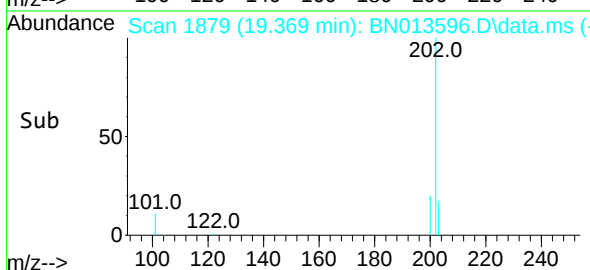
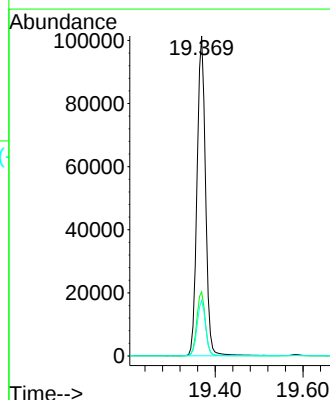
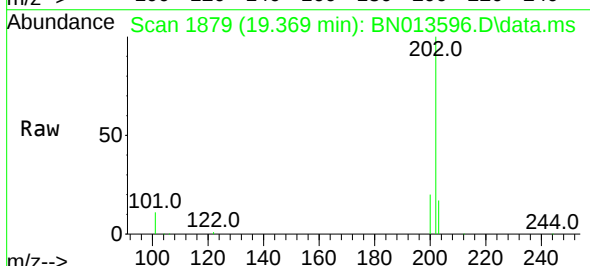




#31
 Terphenyl-d14
 Concen: 1.38 ng
 RT: 19.588 min Scan# 1923
 Delta R.T. 0.000 min
 Lab File: BN013596.D
 Acq: 08 Feb 2021 13:12




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 99312
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.1 9.1
 122 10.5 9.8 14.8

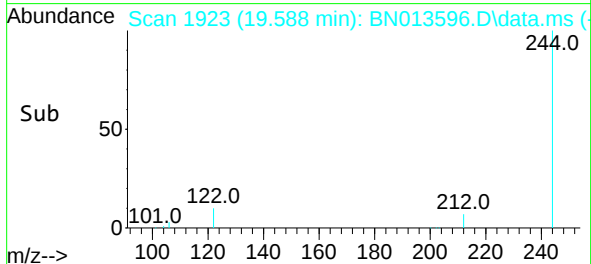

#32
 Benzo(a)anthracene
 Concen: 1.25 ng
 RT: 21.120 min Scan# 2112
 Delta R.T. 0.000 min
 Lab File: BN013596.D
 Acq: 08 Feb 2021 13:12

Tgt Ion:228 Resp: 122537
 Ion Ratio Lower Upper
 228 100
 226 26.4 20.5 30.7
 229 19.3 16.2 24.4

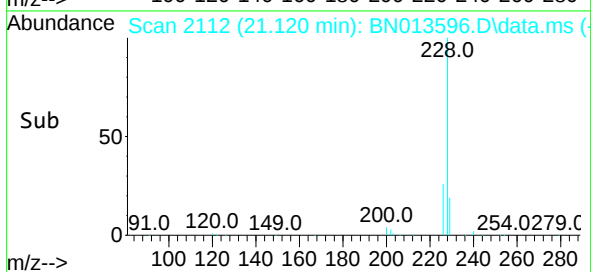

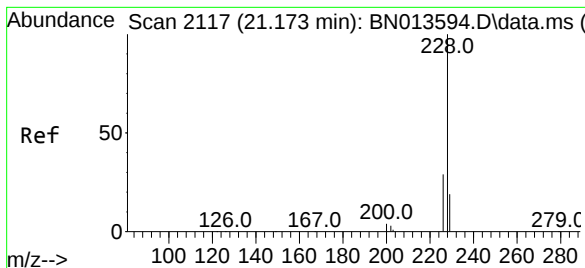

#33

Chrysene

Concen: 1.27 ng

RT: 21.173 min Scan# 2117

Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12

Instrument :

BNA_N

ClientSampleId :

SSTDIC1.6





Tgt Ion:228 Resp: 138225

Ion Ratio Lower Upper

228 100

226 29.2 24.3 36.5

229 19.2 15.1 22.7

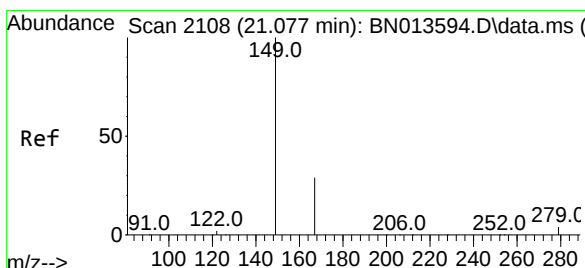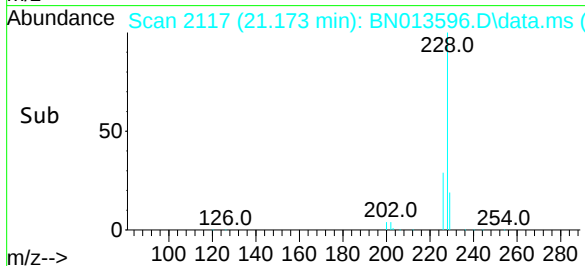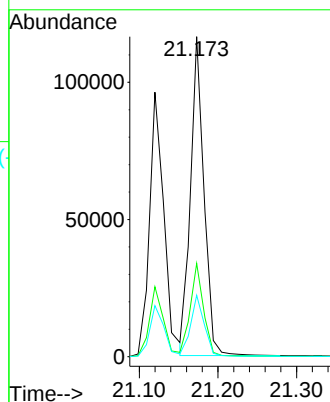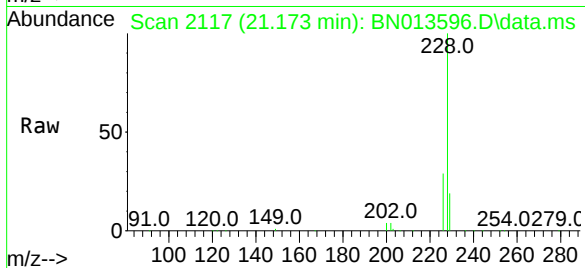

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.07 ng

RT: 21.077 min Scan# 2108

Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12




Tgt Ion:149 Resp: 32480


Ion Ratio Lower Upper

149 100

167 27.5 22.1 33.1

279 4.2 3.5 5.3


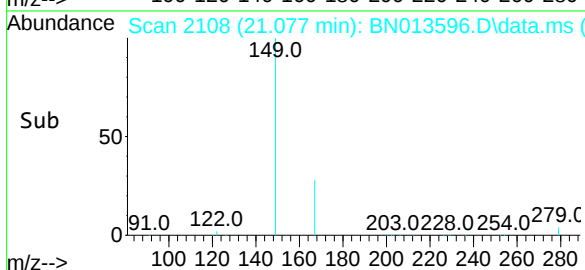
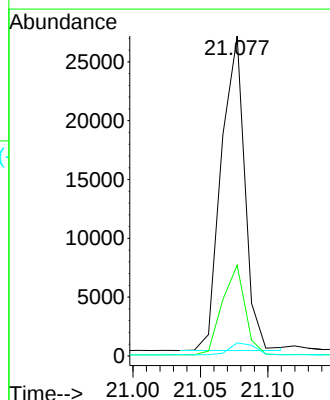
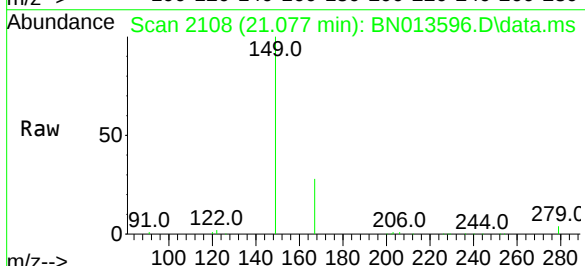




#35
Indeno(1,2,3-cd)pyrene
Concen: 1.28 ng
RT: 25.451 min Scan# 3123
Delta R.T. -0.003 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:276 Resp: 145774
Ion Ratio Lower Upper
276 100
138 26.2 19.8 29.6
277 25.0 19.9 29.9

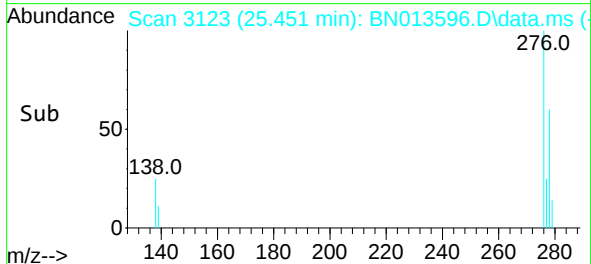

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.305 min Scan# 2496
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:264 Resp: 22788
Ion Ratio Lower Upper
264 100
260 24.8 19.3 28.9
265 34.1 66.2 99.4#


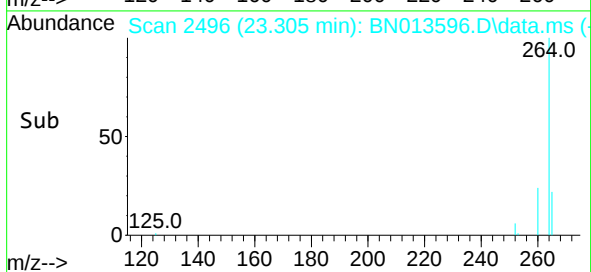






#37
Benzo(b)fluoranthene
Concen: 1.41 ng
RT: 22.662 min Scan# 2308
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 132911
Ion Ratio Lower Upper
252 100
253 22.1 20.4 30.6
125 10.3 11.6 17.4#

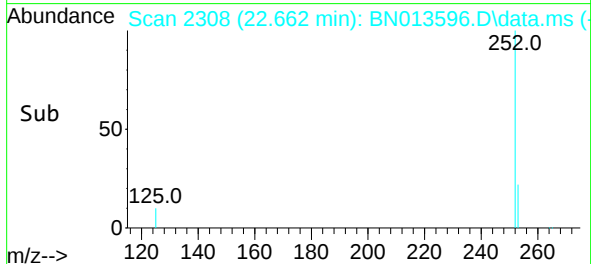

#38
Benzo(k)fluoranthene
Concen: 1.52 ng
RT: 22.703 min Scan# 2320
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Tgt Ion:252 Resp: 139203
Ion Ratio Lower Upper
252 100
253 22.2 20.5 30.7
125 10.5 12.3 18.5#

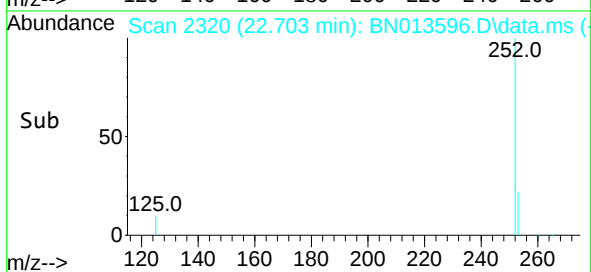



#39

Benzo(a)pyrene

Concen: 1.46 ng

RT: 23.209 min Scan# 2468

Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12





Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6

Tgt Ion:252	Resp:	113481
Ion Ratio	Lower	Upper
252	100	
253	22.5	21.8 32.6
125	11.8	14.6 21.8#

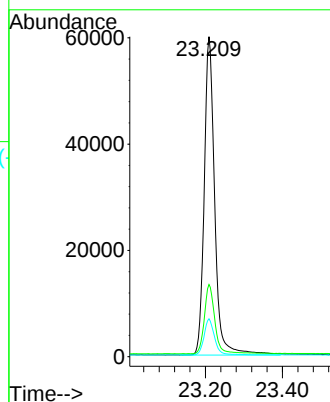

#40

Dibenzo(a,h)anthracene

Concen: 1.44 ng




RT: 25.468 min Scan# 3128


Delta R.T. 0.000 min

Lab File: BN013596.D

Acq: 08 Feb 2021 13:12


Tgt Ion:278	Resp:	125201
Ion Ratio	Lower	Upper
278	100	
139	16.6	13.1 19.7
279	23.9	21.4 32.0

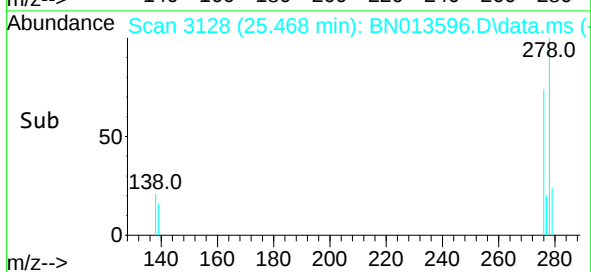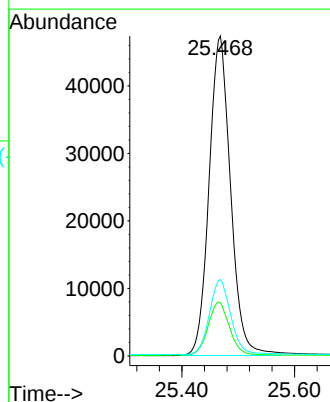

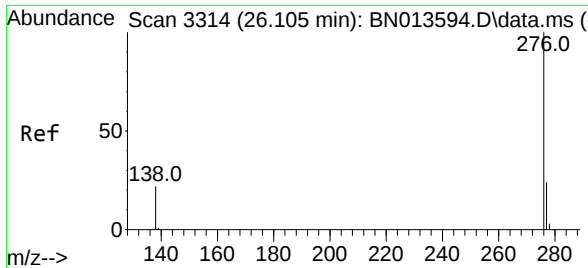

#41
Benzo(g,h,i)perylene
Concen: 1.44 ng
RT: 26.105 min Scan# 3314
Delta R.T. 0.000 min
Lab File: BN013596.D
Acq: 08 Feb 2021 13:12

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

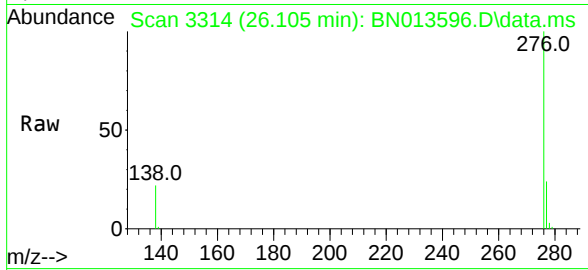

Tgt Ion:276 Resp: 127960
Ion Ratio Lower Upper
276 100
277 23.9 20.0 30.0
138 22.2 17.8 26.8

