


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020821\
 Data File : BN013591.D
 Acq On : 08 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 08 15:13:18 2021

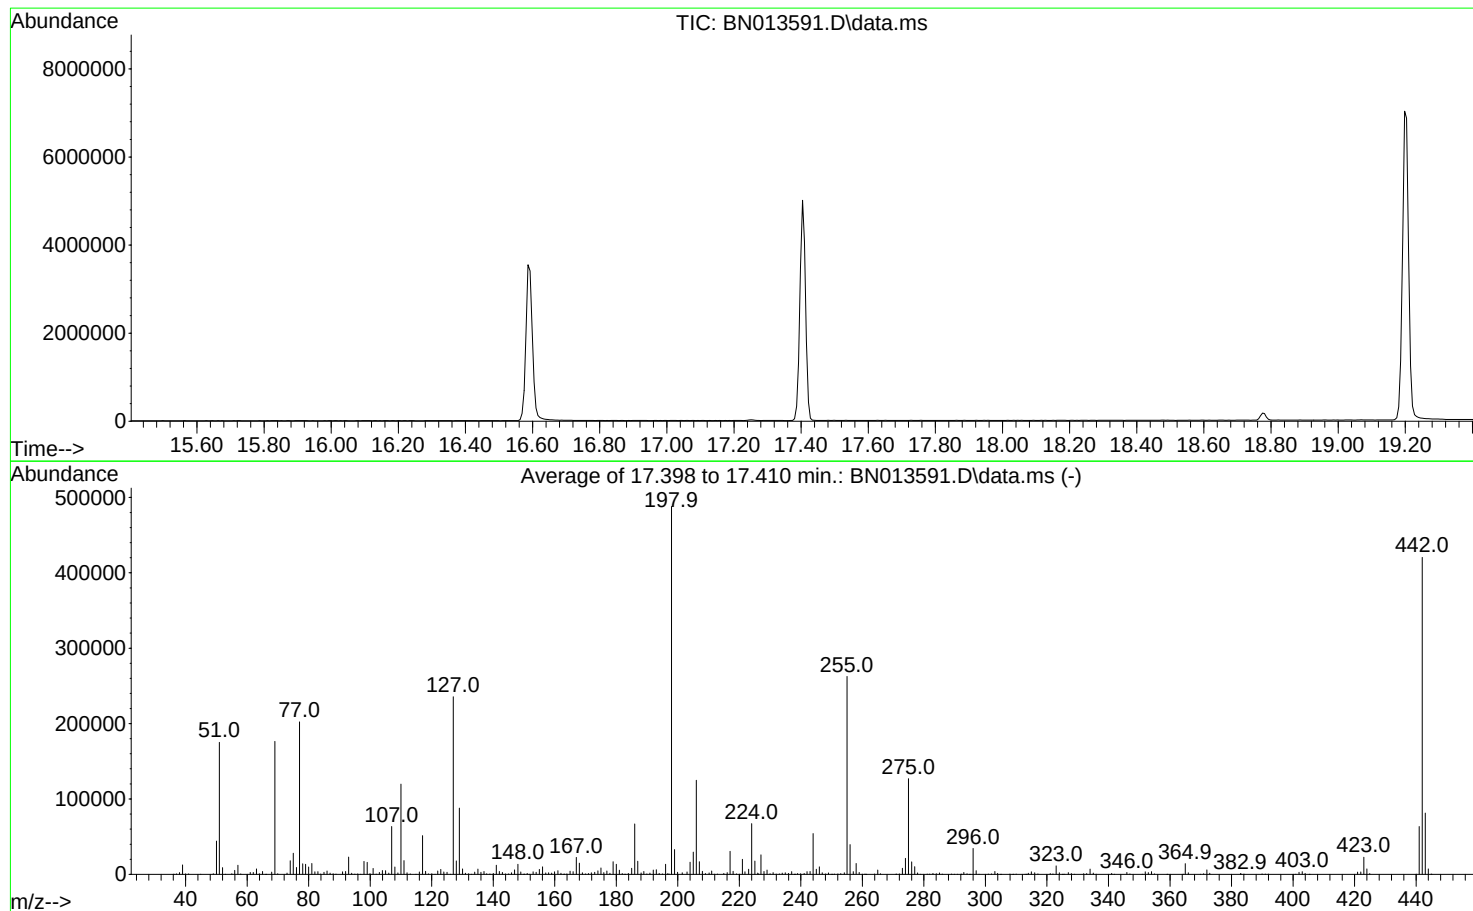




AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2427

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	175120	PASS
68	69	0.00	2	1.7	2917	PASS
69	198	0.00	100	36.1	176384	PASS
70	69	0.00	2	0.5	872	PASS
127	198	10	80	48.3	235520	PASS
197	198	0.00	2	0.2	885	PASS
198	198	100	100	100.0	487979	PASS
199	198	5	9	6.8	32960	PASS
275	198	10	60	26.0	126901	PASS
365	198	1	100	2.9	14151	PASS
441	198	0.01	100	13.0	63440	PASS
442	442	50	100	100.0	420587	PASS
443	442	15	24	19.3	81304	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020821\
Data File : BN013591.D
Acq On : 08 Feb 2021 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 08 16:58:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 08 15:13:18 2021
Response via : Initial Calibration

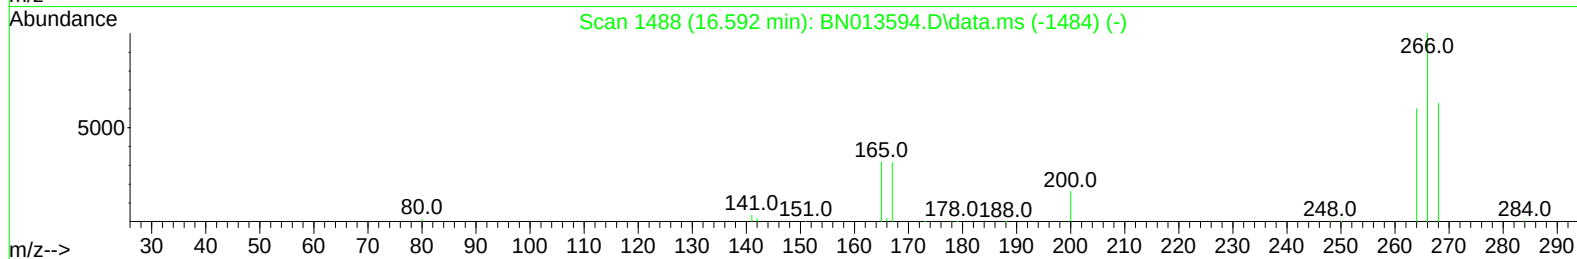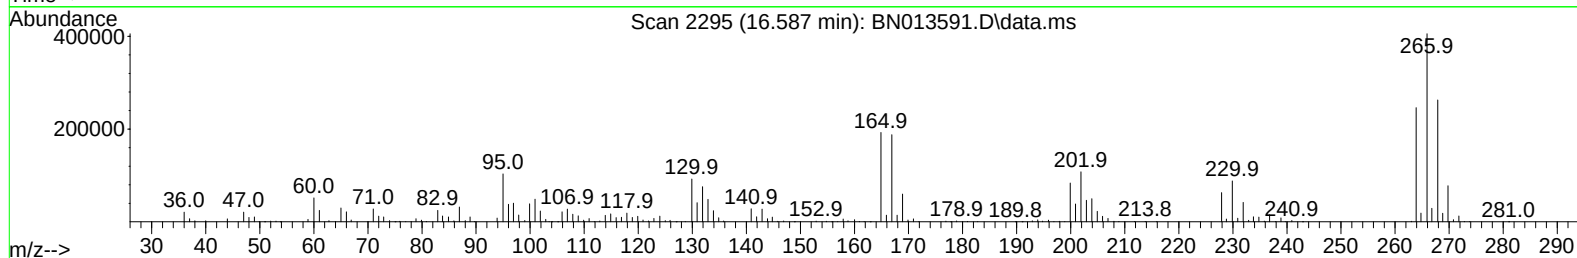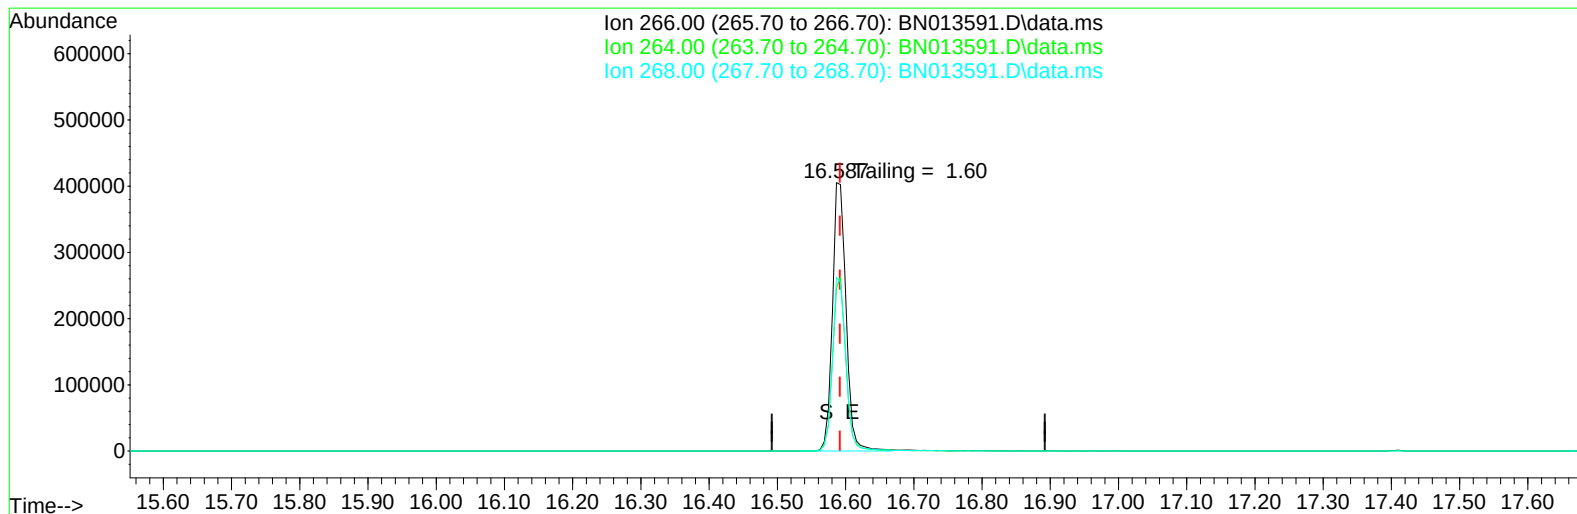

TIC: BN013591.D\data.ms

(24) Pentachlorophenol

16.587min (-0.005) 0.00 ng

response 562853

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.14
268.00	68.30	63.95
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2021	BNA_N	<u>BN013591.D</u>
Compound Name	Response	Retention Time
DDT	1889698	20.44
DDD	5526	20
DDE	2105	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7631	1897329	0.40