
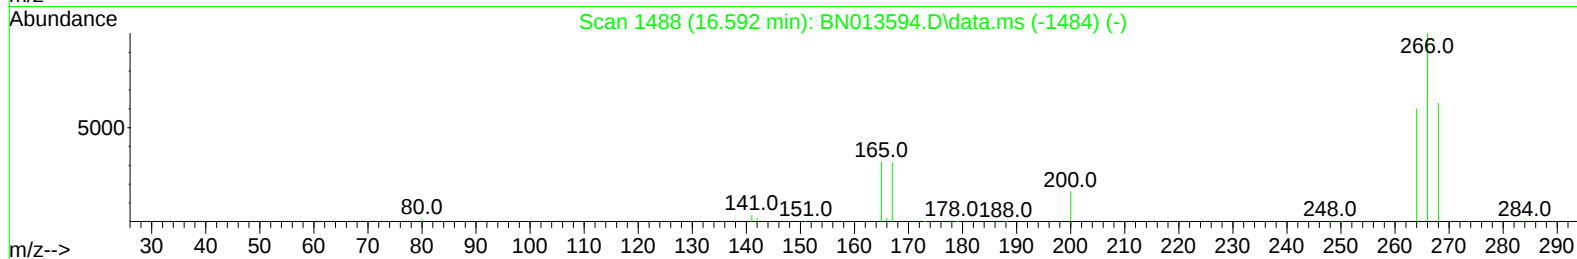
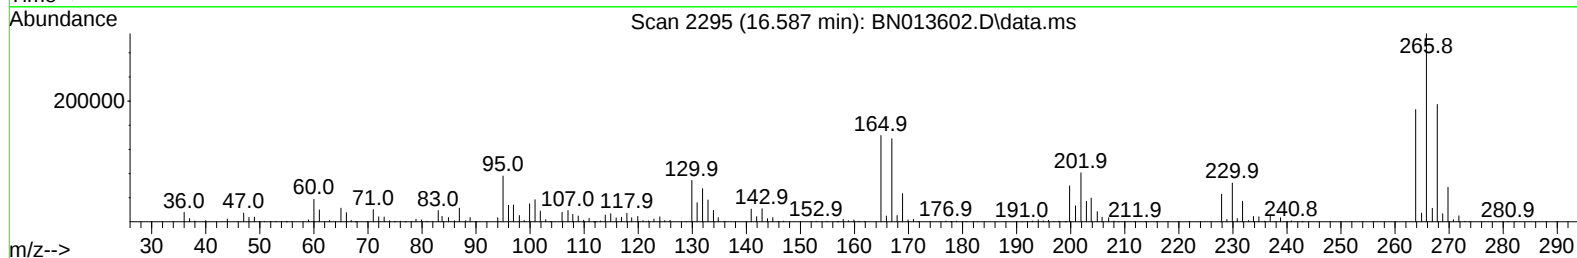


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020921\
Data File : BN013602.D
Acq On : 09 Feb 2021 13:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 15:24:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 08 15:13:18 2021
Response via : Initial Calibration

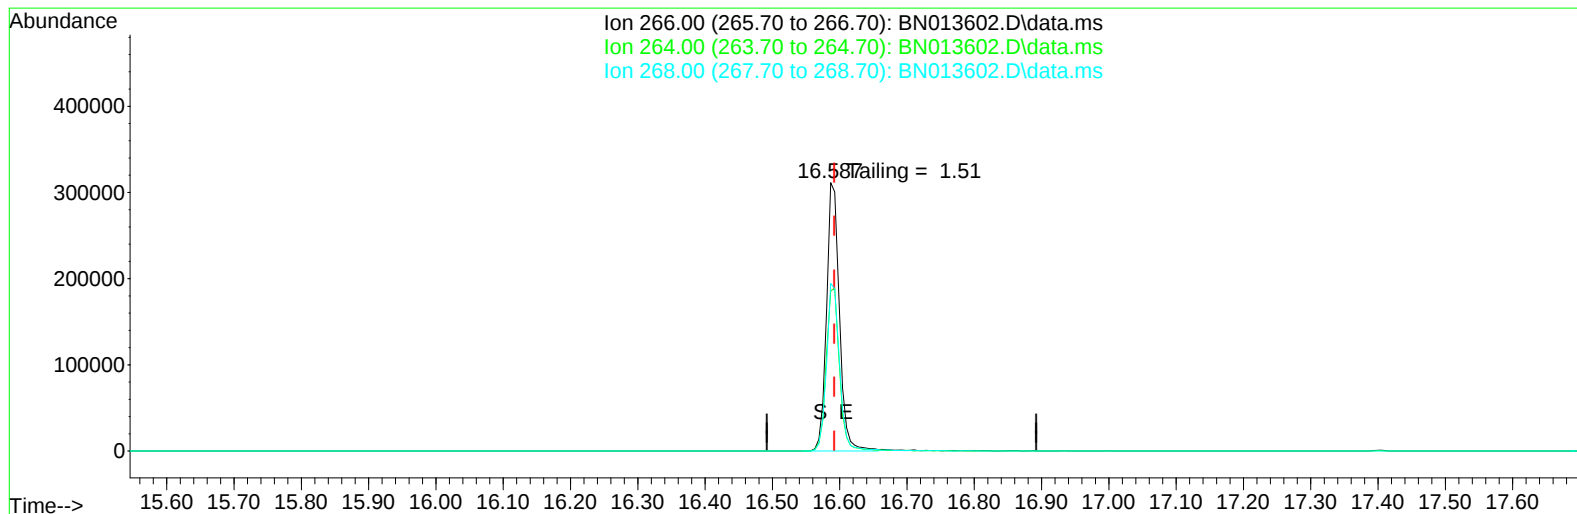

TIC: BN013602.D\data.ms

(24) Pentachlorophenol

16.587min (-0.005) 0.00 ng

response 417045

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	62.40
268.00	68.30	62.98
0.00	0.00	0.00