
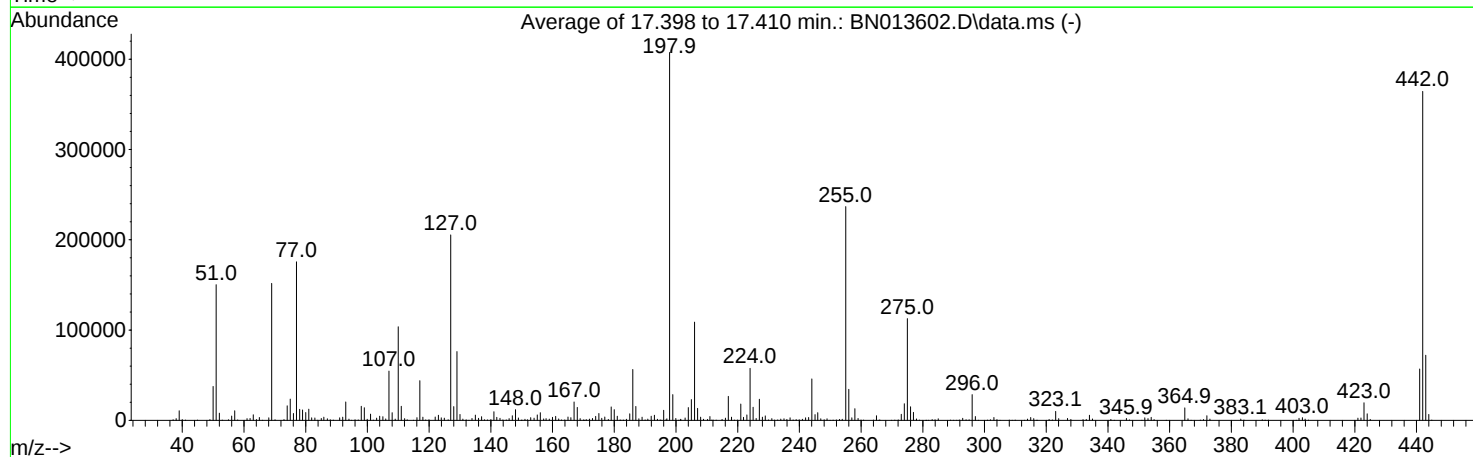


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020921\
 Data File : BN013602.D
 Acq On : 09 Feb 2021 13:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 08 15:13:18 2021

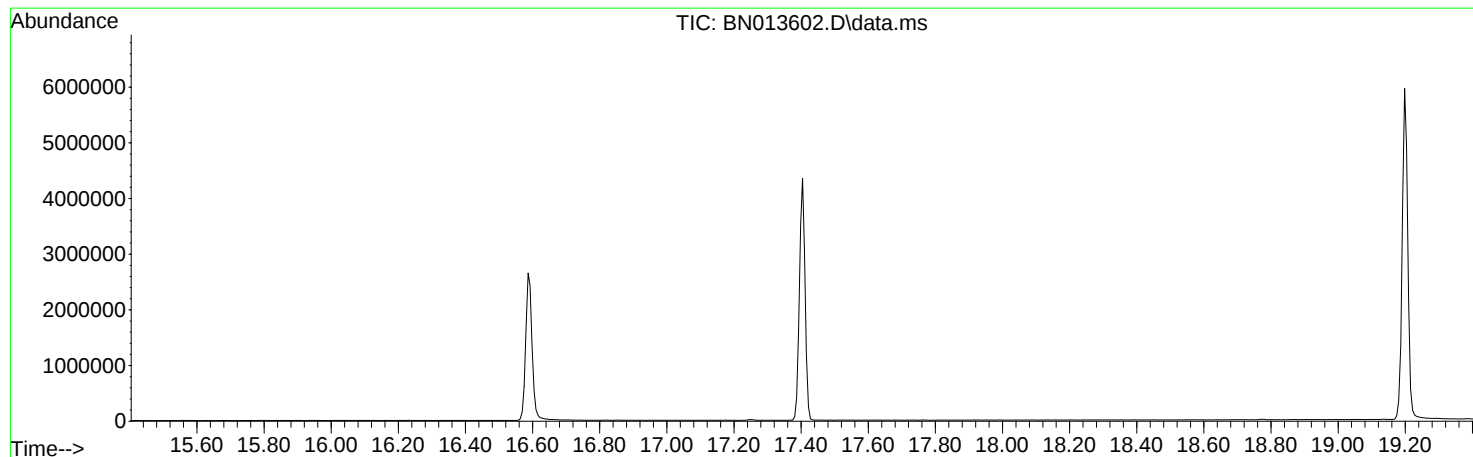




AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	150317	PASS
68	69	0.00	2	1.9	2904	PASS
69	198	0.00	100	37.2	151773	PASS
70	69	0.00	2	0.5	725	PASS
127	198	10	80	50.4	205419	PASS
197	198	0.00	2	0.4	1702	PASS
198	198	100	100	100.0	407445	PASS
199	198	5	9	7.0	28493	PASS
275	198	10	60	27.7	112808	PASS
365	198	1	100	3.4	13833	PASS
441	198	0.01	100	14.0	56843	PASS
442	442	50	100	100.0	364395	PASS
443	442	15	24	19.8	72168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020921\
Data File : BN013602.D
Acq On : 09 Feb 2021 13:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 16 05:41:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

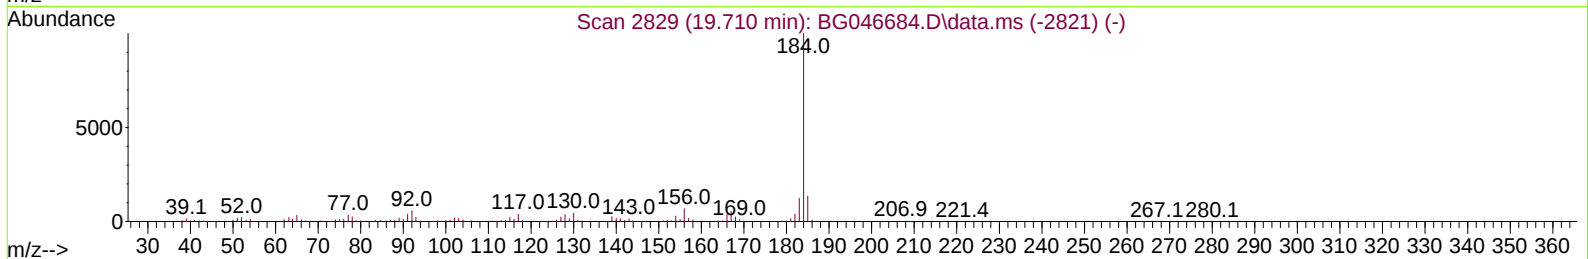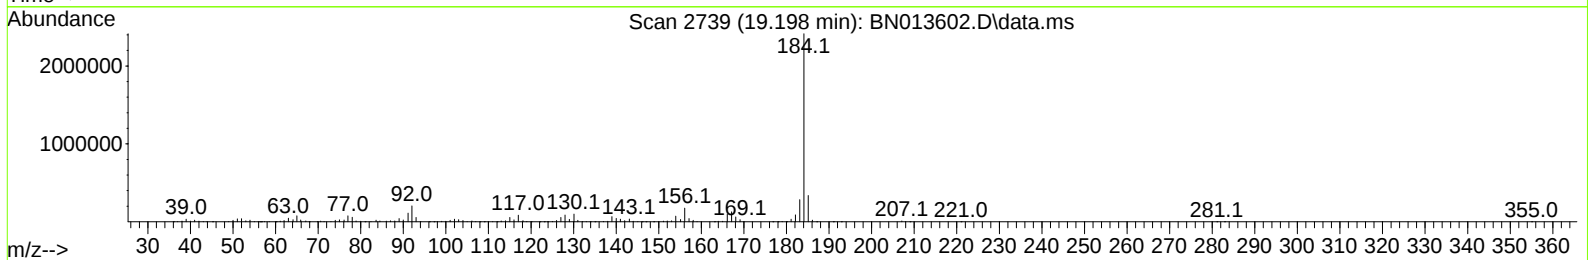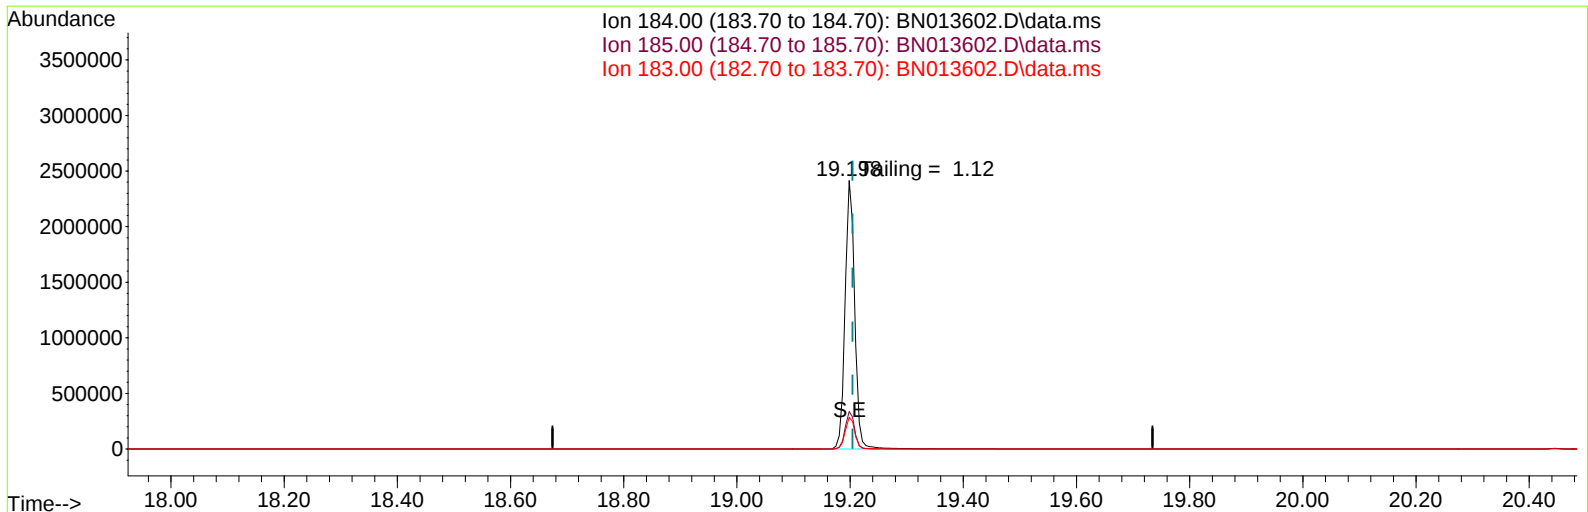

TIC: BN013602.D\data.ms

(77) Benzidine

19.198min (-0.006) 0.00 ng




response 2852062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020921\
 Data File : BN013602.D
 Acq On : 09 Feb 2021 13:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 05:41:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 05:39:20 2021
 Response via : Initial Calibration

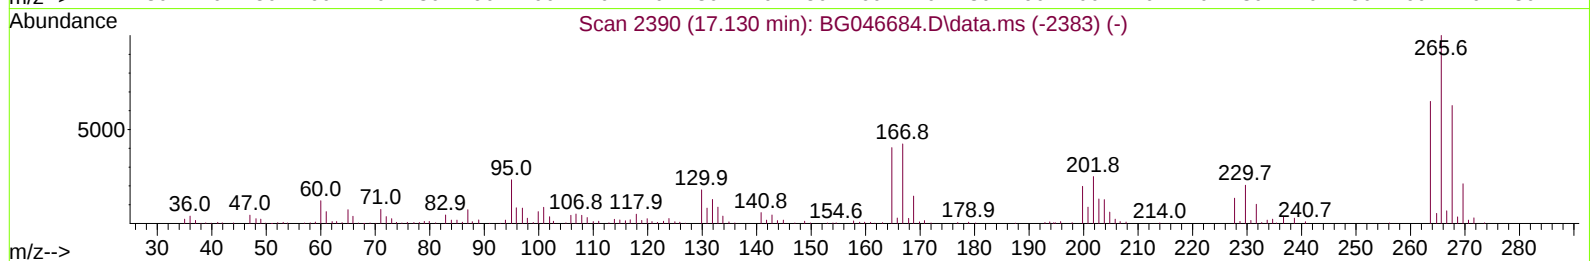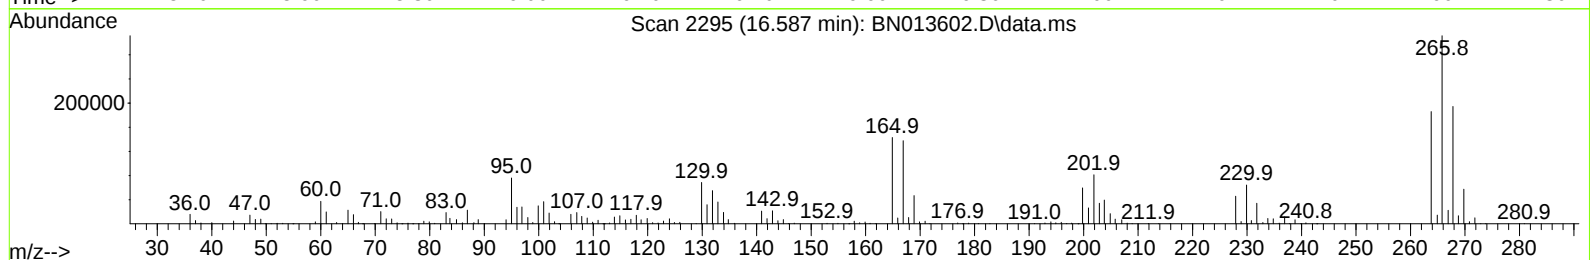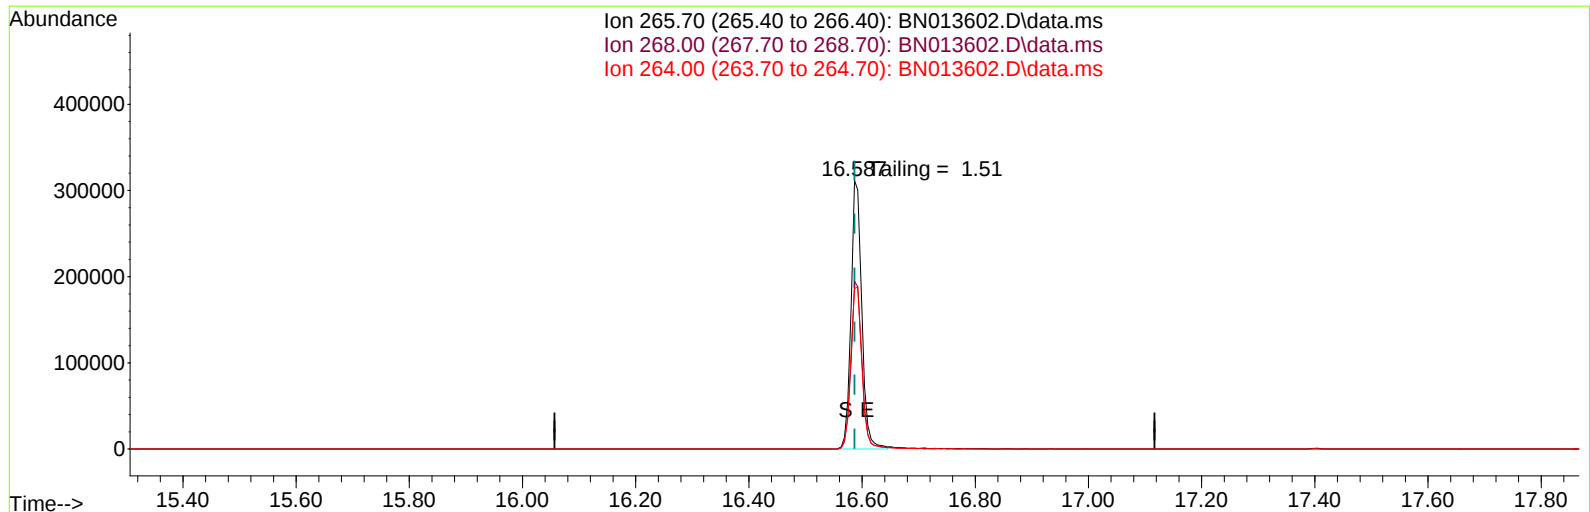

TIC: BN013602.D\data.ms

(70) Pentachlorophenol (C)

16.587min (+ 0.000) 19963.18 ng

response 417045

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.41
264.00	61.60	59.68
0.00	0.00	0.00

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2021	BNA_N	<u>BN013602.D</u>
Compound Name	Response	Retention Time
DDT	1398632	20.44
DDD	5549	20
DDE	1869	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7418	1406050	0.53