

Data File : BN009681.D
Acq On : 10 Feb 2020 12:00
Operator : CG/JU
Sample : PB126689BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK89

Quant Time: Feb 11 01:38:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 15:21:46 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	118136	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.18	136	488606	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.06	164	302828	20.00	ng/ul	-0.01
61) Phenanthrene-d10	16.82	188	639550	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	623185	20.00	ng/ul	0.00
85) Perylene-d12	23.15	264	610138	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	18844	6.54	ng/uL	0.00
5) Phenol-d5	6.62	99	356388	34.59	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.78	67	247411	35.75	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	279480	36.85	ng/ul	-0.01
13) 4-Methylphenol-d8	8.13	113	278081	33.89	ng/ul	-0.01
19) Nitrobenzene-d5	8.57	128	134840	37.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	150835	37.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.81	165	267052	35.15	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.32	131	376112	46.05	ng/ul	-0.01
43) Dimethylphthalate-d6	13.49	166	808442	36.57	ng/ul	0.00
46) Acenaphthylene-d8	13.75	160	973654	36.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	120539	28.87	ng/ul	0.00
57) Fluorene-d10	15.07	176	712953	36.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	102415	25.64	ng/ul	0.00
70) Anthracene-d10	16.92	188	1079364	37.14	ng/ul	0.00
78) Pyrene-d10	19.23	212	1129696	34.48	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	1157904	38.54	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.13	70	7994	1.150	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009681.D
Acq On : 10 Feb 2020 12:00
Operator : CG/JU
Sample : PB126689BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK89

Quant Time: Feb 11 01:38:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 15:21:46 2020
Response via : Initial Calibration

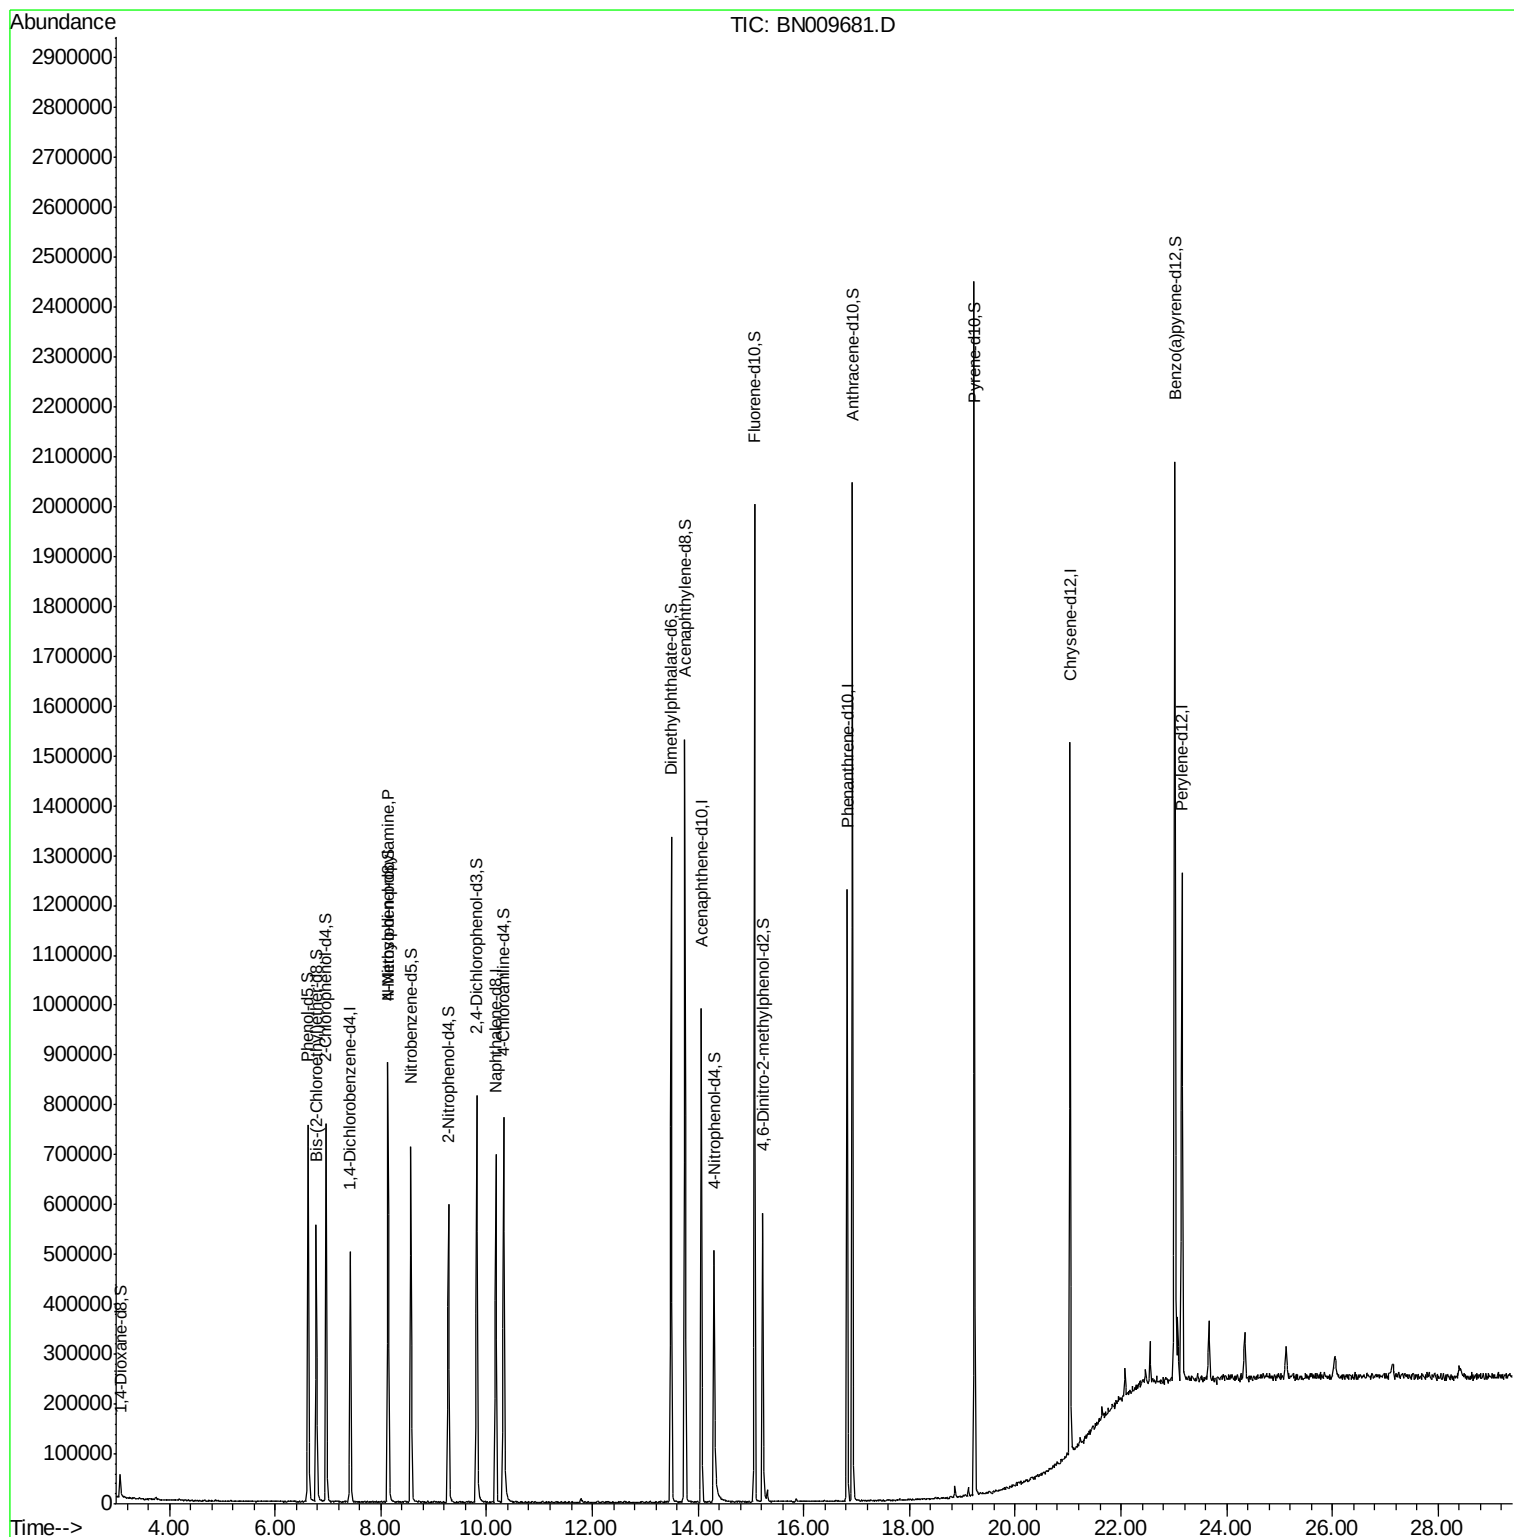

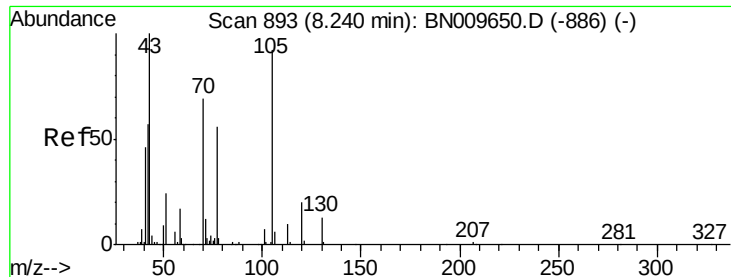

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.150 ng/ul
 RT: 8.13 min Scan# 875
 Delta R.T. -0.11 min
 Lab File: BN009681.D
 Acq: 10 Feb 2020 12:00

Instrument :
 BNA_N
 ClientSampleId :
 SBLK89

Tgt Ion: 70 Resp: 7994
 Ion Ratio Lower Upper
 70 100
 42 560.2 68.3 102.5#
 101 0.0 7.4 11.0#
 130 0.0 14.2 21.2#

