

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021020\
 Data File : BN009696.D
 Acq On : 10 Feb 2020 21:36
 Operator : CG/JU
 Sample : L1324-16MEDL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT71MEDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	65	67	70	rVB3	2218	2259	0.12%	0.023%
2	3.464	79	81	84	rBV3	2839	3393	0.17%	0.034%
3	3.705	120	122	126	rBV4	2681	3813	0.20%	0.038%
4	3.752	126	130	135	rVV4	5380	9066	0.47%	0.091%
5	3.846	144	146	149	rVB4	2581	2201	0.11%	0.022%
6	3.934	159	161	165	rVB4	1618	2291	0.12%	0.023%
7	4.916	326	328	331	rVB2	2556	2680	0.14%	0.027%
8	4.940	331	332	335	rBV3	1810	1994	0.10%	0.020%
9	4.987	338	340	343	rVV4	2157	2442	0.13%	0.025%
10	5.040	348	349	352	rVB3	2883	2458	0.13%	0.025%
11	5.211	374	378	380	rBV3	1953	2333	0.12%	0.024%
12	5.246	382	384	386	rBV3	2047	2314	0.12%	0.023%
13	5.522	428	431	435	rBV4	1607	2630	0.14%	0.027%
14	5.593	440	443	447	rVB3	2104	2695	0.14%	0.027%
15	5.663	453	455	457	rVB2	2834	2357	0.12%	0.024%
16	6.063	521	523	526	rBV3	1884	2002	0.10%	0.020%
17	6.375	572	576	577	rVB3	1828	2386	0.12%	0.024%
18	7.287	728	731	736	rBV4	2044	2465	0.13%	0.025%
19	7.428	749	755	768	rVV	520882	843136	43.32%	8.504%
20	7.657	792	794	797	rBV3	1952	2131	0.11%	0.021%
21	7.810	817	820	824	rVB3	1526	2141	0.11%	0.022%
22	8.181	881	883	886	rVB	2348	2424	0.12%	0.024%
23	9.093	1036	1038	1042	rBV3	1497	2031	0.10%	0.020%
24	10.087	1205	1207	1211	rVB3	2212	2028	0.10%	0.020%
25	10.122	1211	1213	1215	rBV3	1743	2141	0.11%	0.022%
26	10.181	1215	1223	1236	rBV	674790	1197971	61.56%	12.083%
27	10.487	1271	1275	1277	rBV	1887	2441	0.13%	0.025%
28	10.710	1309	1313	1315	rVB4	1932	2101	0.11%	0.021%
29	10.793	1323	1327	1331	rVB4	1765	2135	0.11%	0.022%
30	11.457	1437	1440	1441	rBV3	1776	1963	0.10%	0.020%
31	12.569	1628	1629	1635	rVB2	1780	2393	0.12%	0.024%
32	12.628	1635	1639	1643	rBV3	2210	3056	0.16%	0.031%
33	13.357	1761	1763	1766	rBV2	1467	1949	0.10%	0.020%
34	13.440	1774	1777	1781	rVV4	1504	2230	0.11%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021020\
 Data File : BN009696.D
 Acq On : 10 Feb 2020 21:36
 Operator : CG/JU
 Sample : L1324-16MEDL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT71MEDL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Title : SVOA CALIBRATION

35	13.757	1828	1831	1832	rVB3	2277	1994	0.10%	0.020%
36	13.787	1832	1836	1837	rBV3	1945	2560	0.13%	0.026%
37	14.069	1877	1884	1895	rBV	995065	1546369	79.46%	15.597%
38	14.263	1916	1917	1920	rBV3	2036	1985	0.10%	0.020%
39	14.339	1928	1930	1935	rVB3	2424	3578	0.18%	0.036%
40	15.228	2078	2081	2083	rBV2	1768	1961	0.10%	0.020%
41	15.422	2109	2114	2116	rBV4	2059	3686	0.19%	0.037%
42	15.610	2144	2146	2149	rVB3	2041	2023	0.10%	0.020%
43	15.810	2177	2180	2182	rVB4	1881	2082	0.11%	0.021%
44	15.898	2194	2195	2198	rBV3	2097	1964	0.10%	0.020%
45	15.934	2198	2201	2202	rBV2	2299	2080	0.11%	0.021%
46	16.298	2261	2263	2268	rBV3	1768	2289	0.12%	0.023%
47	16.557	2304	2307	2310	rBV4	2393	2478	0.13%	0.025%
48	16.610	2310	2316	2320	rVV4	3281	6340	0.33%	0.064%
49	16.822	2346	2352	2373	rBV	1145370	1774916	91.20%	17.902%
50	17.133	2401	2405	2407	rBV3	2750	3175	0.16%	0.032%
51	17.339	2437	2440	2442	rBV3	1948	2753	0.14%	0.028%
52	17.480	2462	2464	2466	rVB2	2438	2033	0.10%	0.021%
53	17.516	2466	2470	2472	rBV4	1184	2048	0.11%	0.021%
54	17.545	2474	2475	2478	rVB3	2761	2673	0.14%	0.027%
55	17.645	2489	2492	2493	rVB3	2258	1983	0.10%	0.020%
56	17.775	2510	2514	2516	rBV4	3166	2109	0.11%	0.021%
57	17.816	2516	2521	2523	rBV4	1396	2585	0.13%	0.026%
58	18.269	2596	2598	2600	rBV2	2081	2274	0.12%	0.023%
59	18.375	2615	2616	2618	rBV2	2271	2023	0.10%	0.020%
60	18.451	2628	2629	2633	rBV2	3248	3798	0.20%	0.038%
61	18.686	2668	2669	2671	rVB2	3323	2243	0.12%	0.023%
62	18.704	2671	2672	2675	rBV2	2449	2306	0.12%	0.023%
63	18.910	2703	2707	2709	rBV3	3212	4199	0.22%	0.042%
64	18.933	2709	2711	2713	rVB3	3362	2523	0.13%	0.025%
65	19.004	2722	2723	2726	rVB3	3313	2298	0.12%	0.023%
66	19.180	2751	2753	2755	rBV3	2755	3085	0.16%	0.031%
67	19.363	2782	2784	2786	rBV3	4228	3613	0.19%	0.036%
68	19.469	2800	2802	2805	rBV2	3655	2971	0.15%	0.030%
69	19.763	2850	2852	2853	rBV2	6501	4121	0.21%	0.042%
70	21.033	3063	3068	3076	rBV	1489773	1946150	100.00%	19.629%
71	22.074	3242	3245	3249	rVB	76500	95583	4.91%	0.964%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021020\
Data File : BN009696.D
Acq On : 10 Feb 2020 21:36
Operator : CG/JU
Sample : L1324-16MEDL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT71MEDL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Title : SVOA CALIBRATION

72	22.545	3322	3325	3332	rVB	95459	137599	7.07%	1.388%
73	23.068	3411	3414	3419	rVB	123302	172795	8.88%	1.743%
74	23.145	3421	3427	3436	rBV	1033421	1875207	96.35%	18.914%
75	23.663	3512	3515	3520	rVB	105485	152080	7.81%	1.534%


Sum of corrected areas: 9914582

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021020\
Data File : BN009696.D
Acq On : 10 Feb 2020 21:36
Operator : CG/JU
Sample : L1324-16MEDL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT71MEDL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

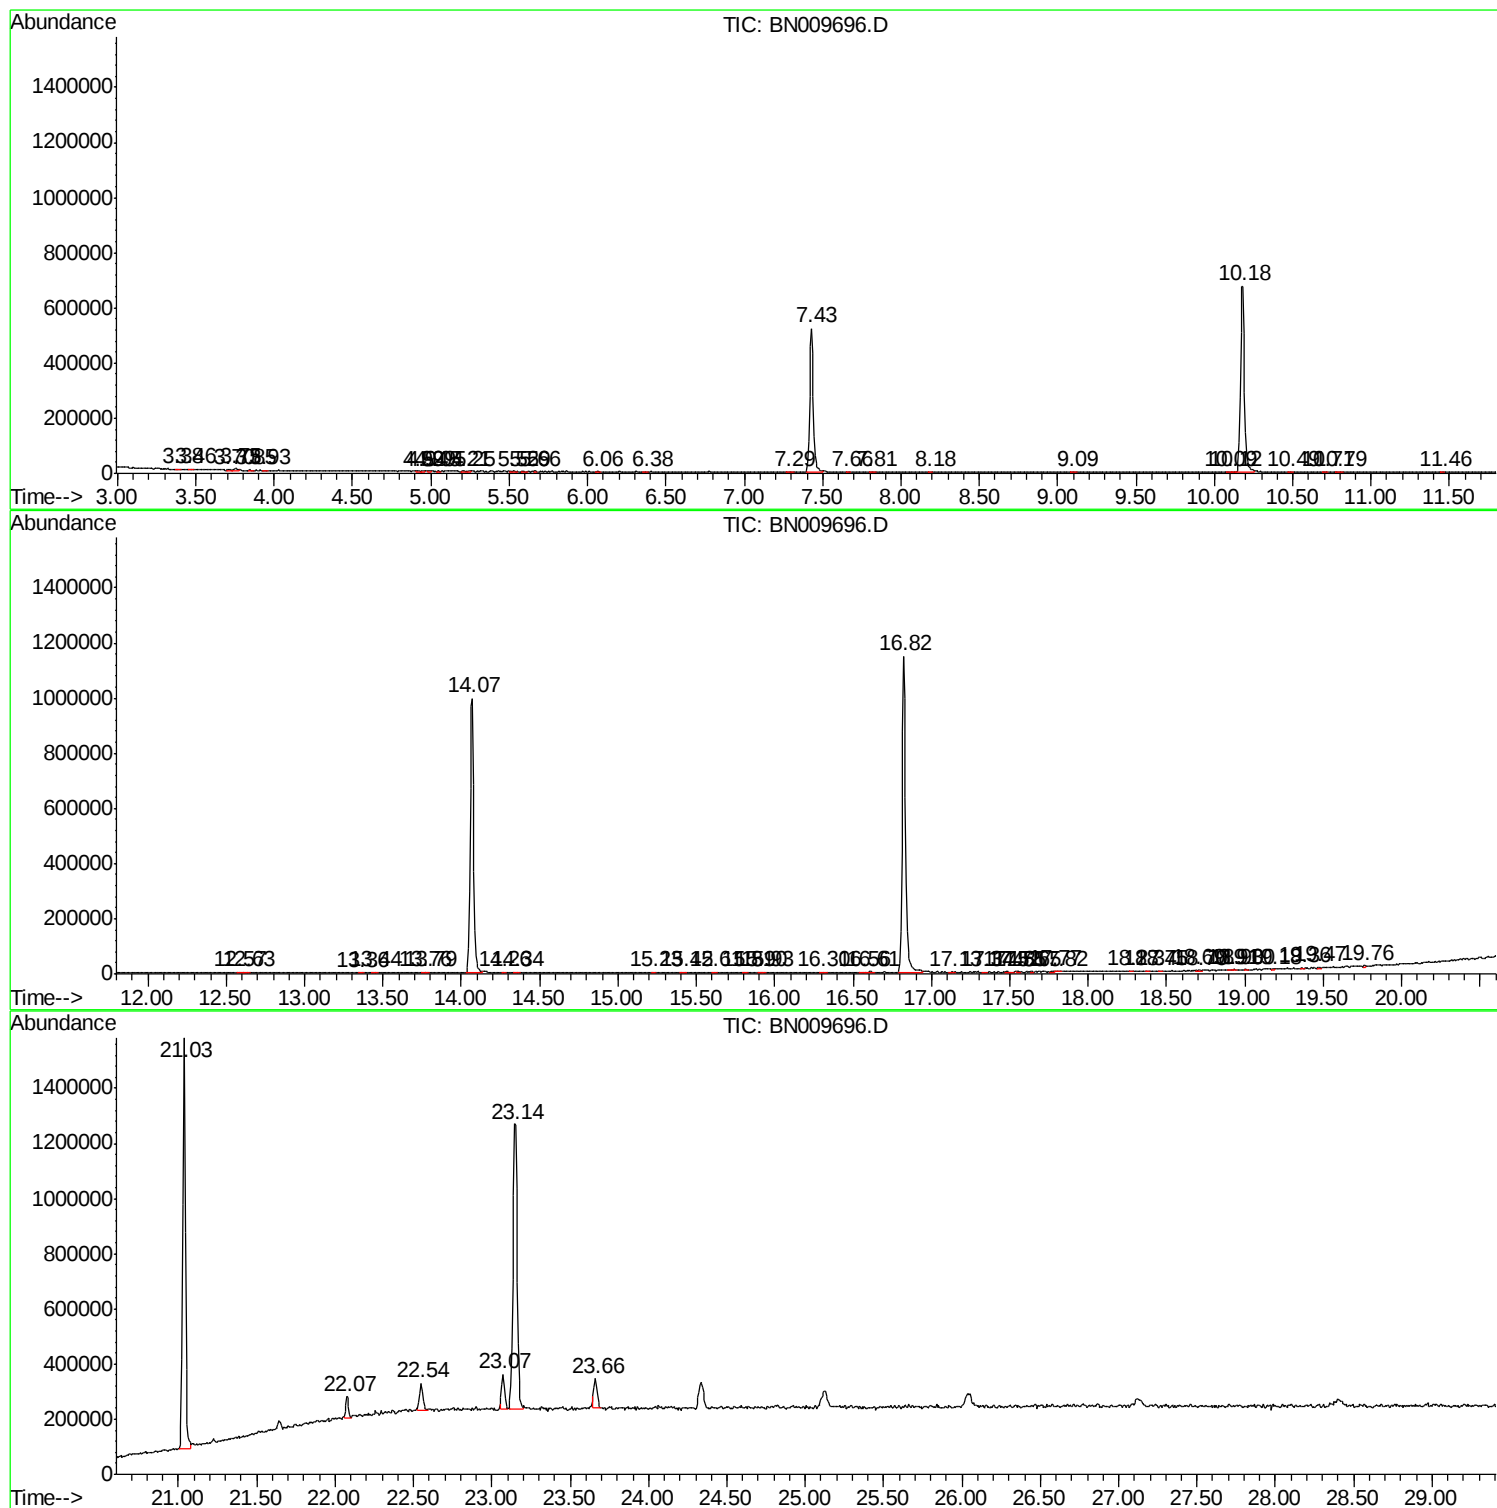

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021020\
Data_File : BN009696.D
Acq_On : 10_Feb_2020 21:366
Operator : CG/JUU
Sample : L1324-16MEDL_10XX
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
GAT71MEDL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
