
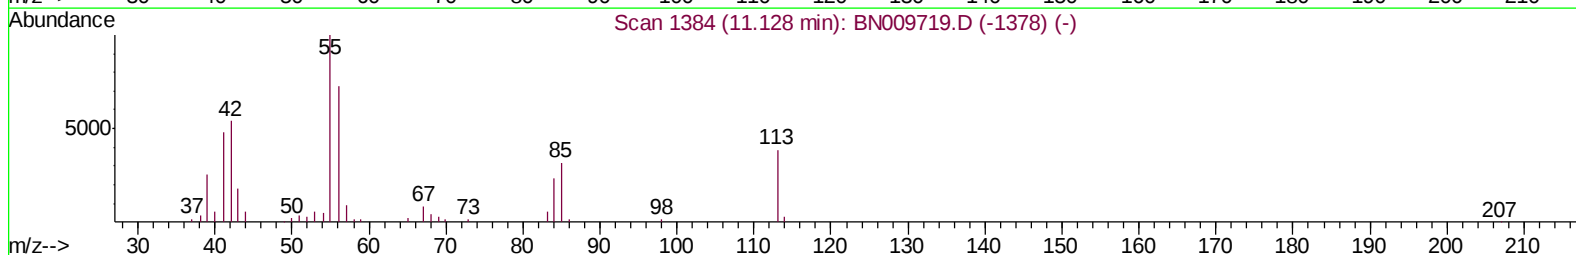
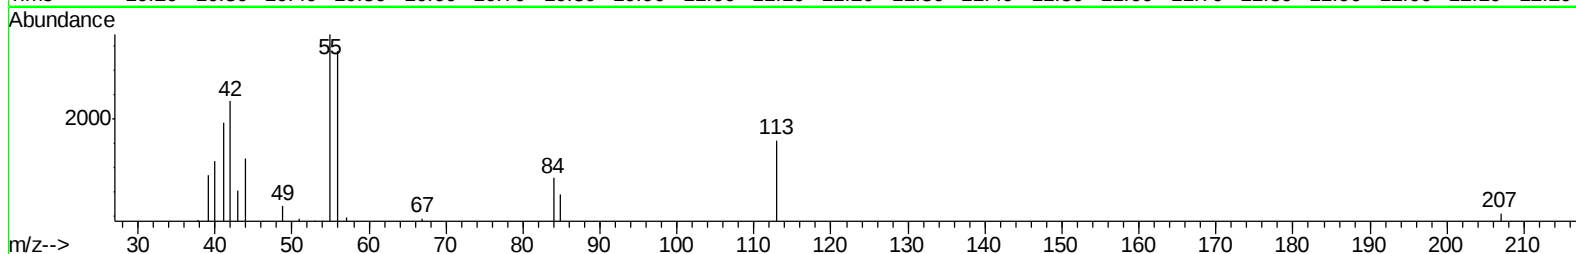


Data File : BN009721.D
Acq On : 14 Feb 2020 12:25
Operator : CG/JU
Sample : K5695-08
Misc : MDL-WATER-01
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Feb 17 00:50:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

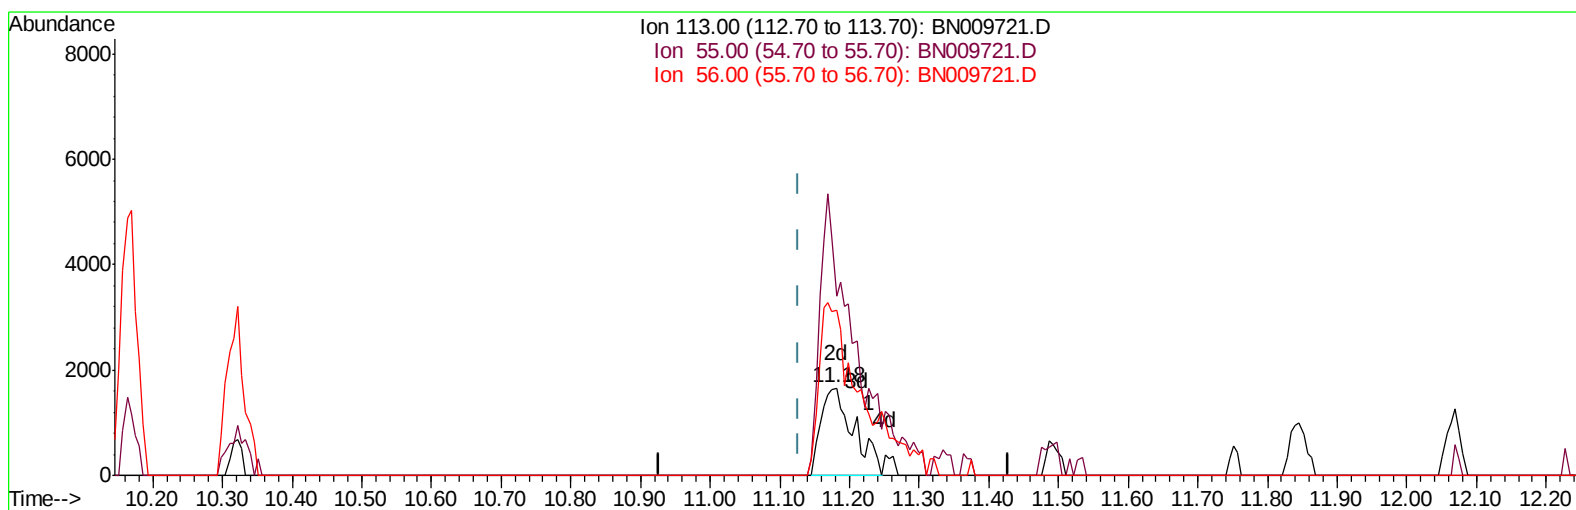

TIC: BN009721.D

(32) Caprolactam

11.181min (+0.053) 2.57ng/ul m

response 5361

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	205.57#
56.00	202.00	189.35
0.00	0.00	0.00