

Data File : BN009722.D

Acq On : 14 Feb 2020 13:01

Operator : CG/JU

Sample : K5695-09

Misc : MDL-WATER-02

ALS Vial : 5 Sample Multiplier: 1




Quant Time: Feb 17 00:50:41 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Feb 17 00:47:25 2020

Response via : Initial Calibration

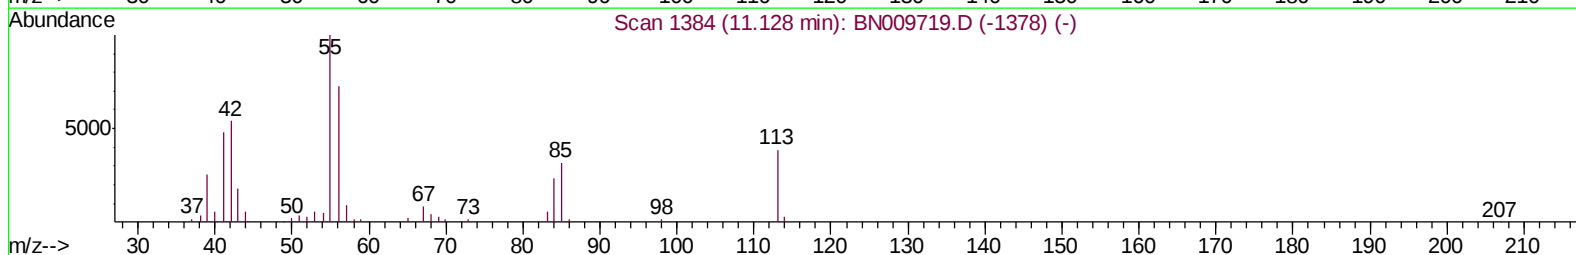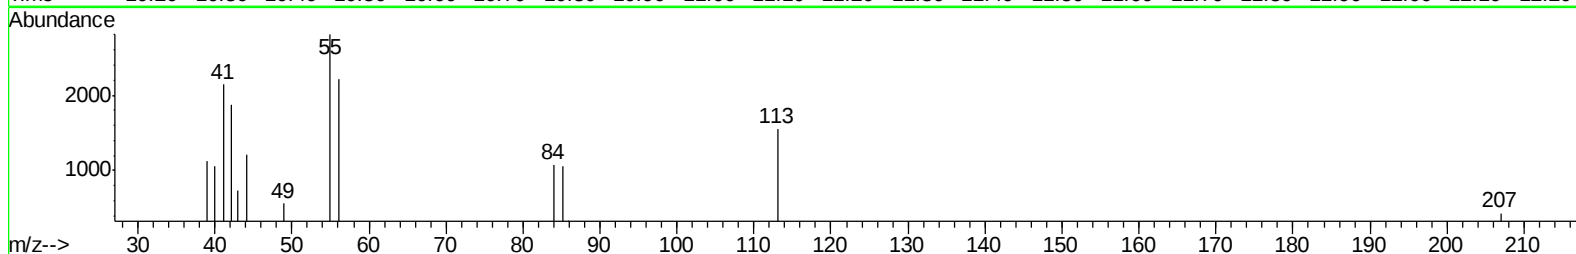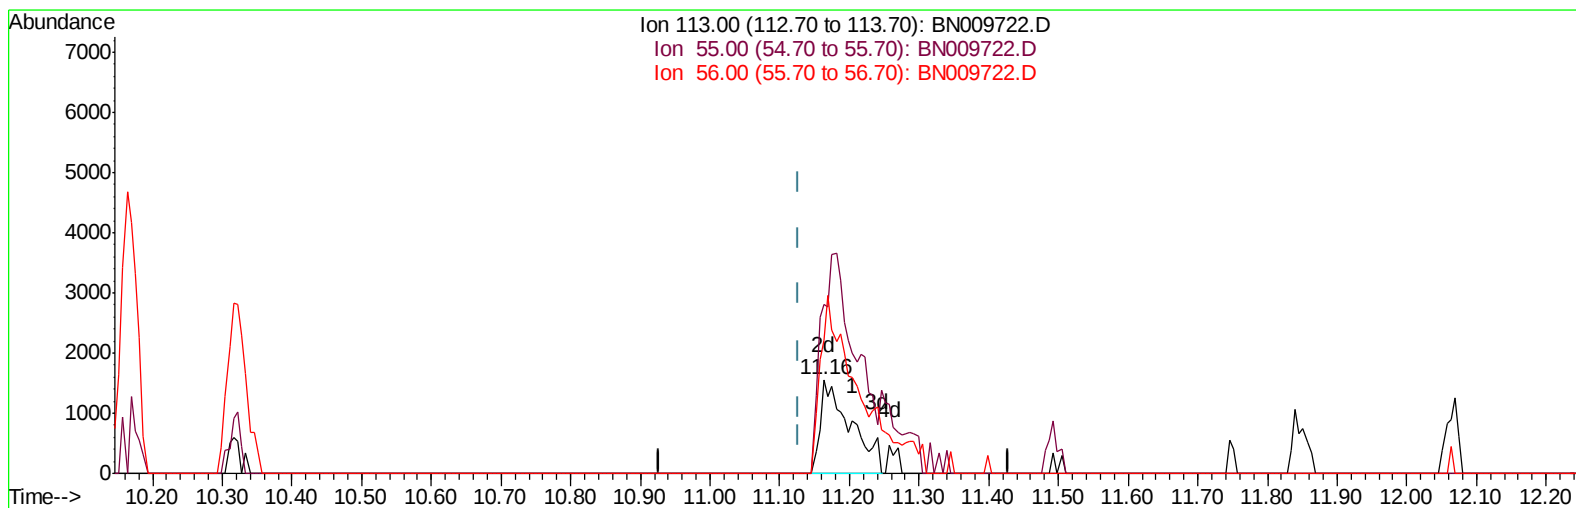

TIC: BN009722.D

(32) Caprolactam

11.163min (+0.035) 2.18ng/ul m

response 4627

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	180.63#
56.00	202.00	142.86#
0.00	0.00	0.00