
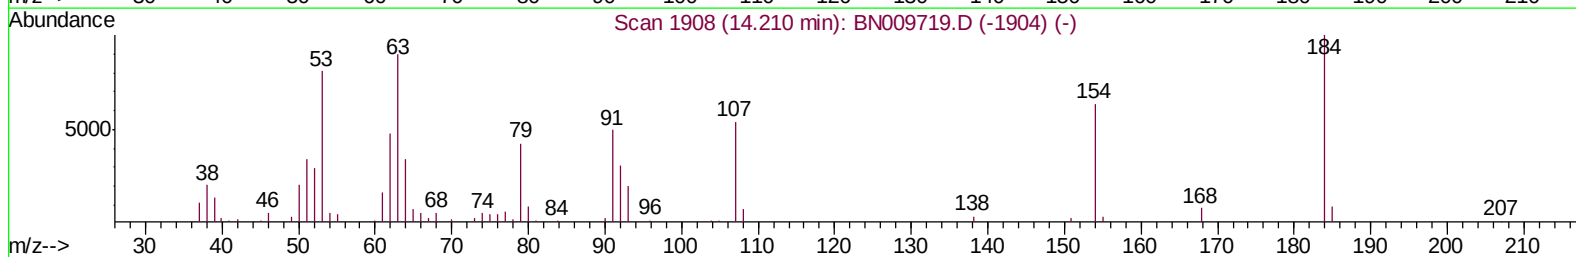
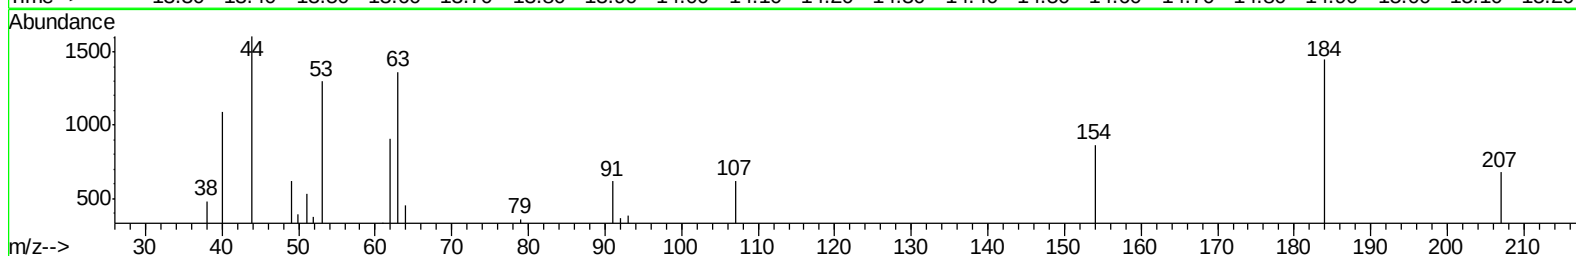


Data File : BN009722.D
Acq On : 14 Feb 2020 13:01
Operator : CG/JU
Sample : K5695-09
Misc : MDL-WATER-02
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 17 00:50:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

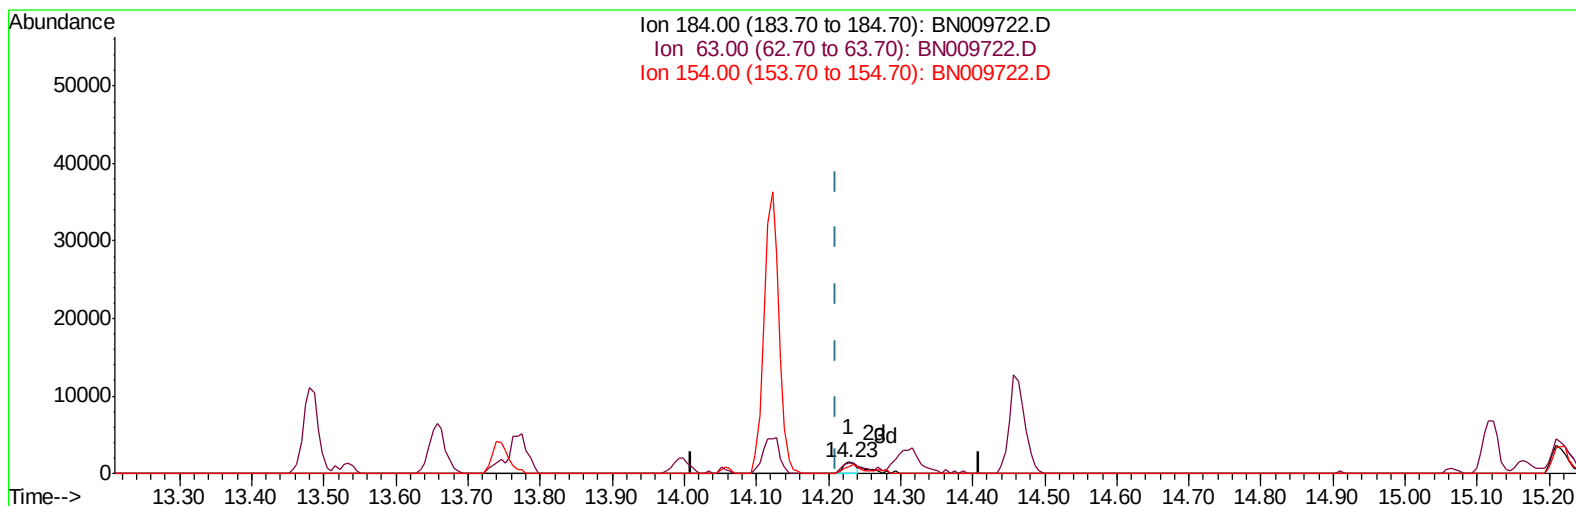

TIC: BN009722.D

(51) 2,4-Dinitrophenol

14.228min (+0.018) 0.74ng/ul

response 1742

Ion	Exp%	Act%
184.00	100	100
63.00	103.80	94.13
154.00	68.60	59.71
0.00	0.00	0.00