

Data File : BN009724.D

Acq On : 14 Feb 2020 14:13

Operator : CG/JU

Sample : K5695-11

Misc : MDL-WATER-04

ALS Vial : 7 Sample Multiplier: 1




Quant Time: Feb 17 00:51:57 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Feb 17 00:47:25 2020

Response via : Initial Calibration

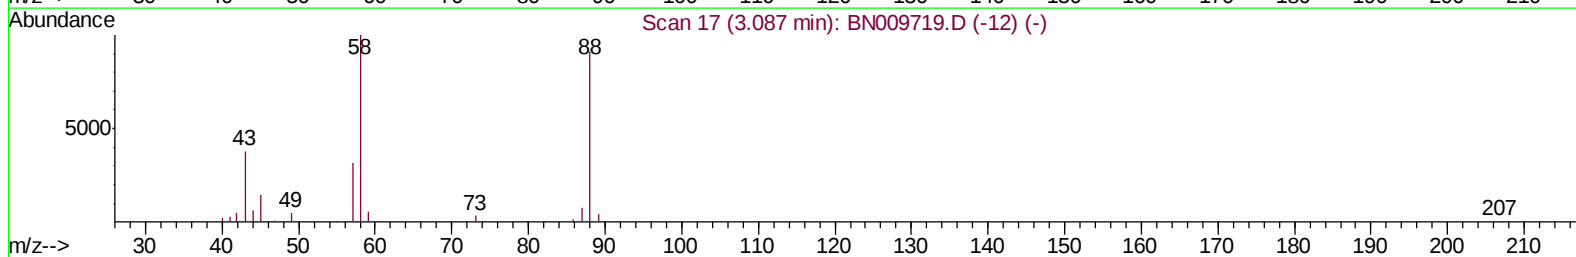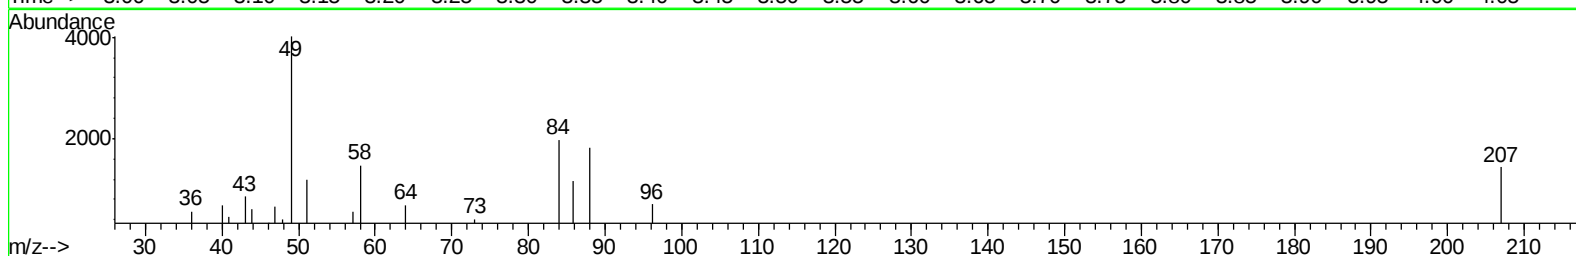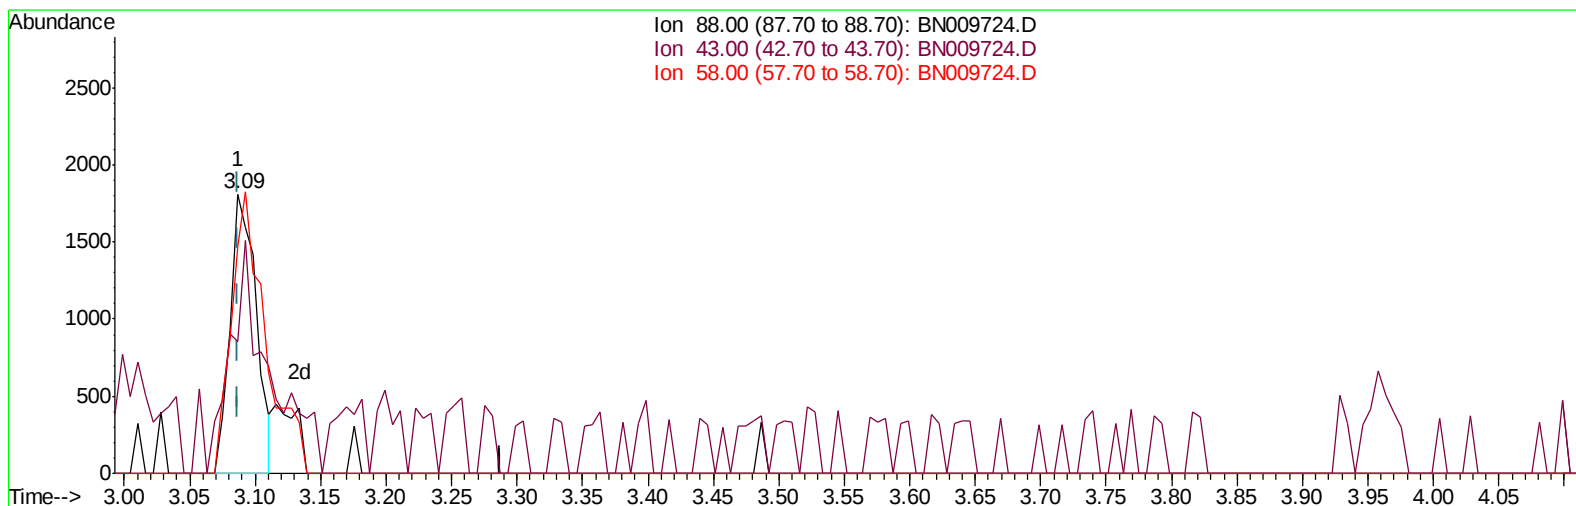

TIC: BN009724.D

(2) 1,4-Dioxane

3.087min (-0.000) 0.86ng/uL

response 2519

Ion	Exp%	Act%
88.00	100	100
43.00	55.90	47.10
58.00	120.20	81.32#
0.00	0.00	0.00