
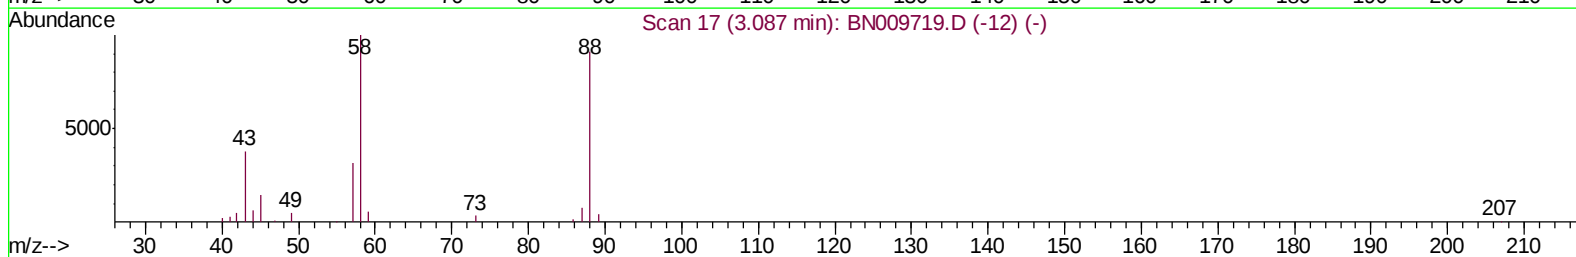
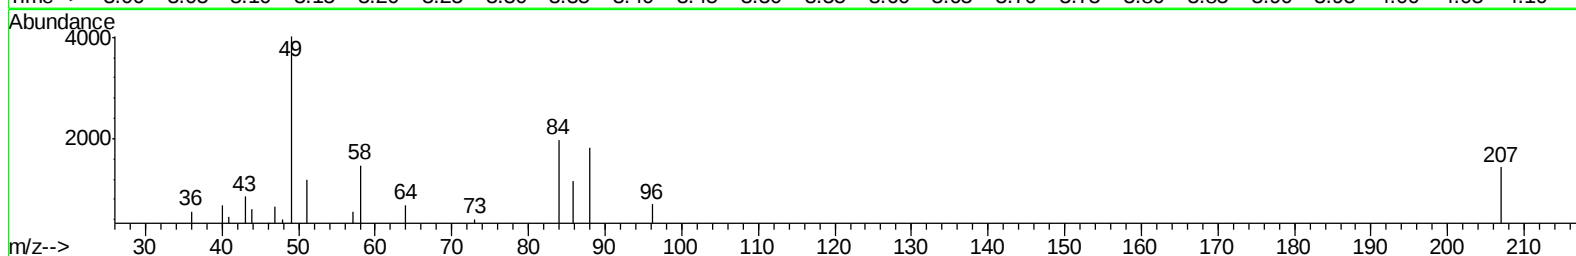


Data File : BN009724.D
Acq On : 14 Feb 2020 14:13
Operator : CG/JU
Sample : K5695-11
Misc : MDL-WATER-04
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 17 00:51:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

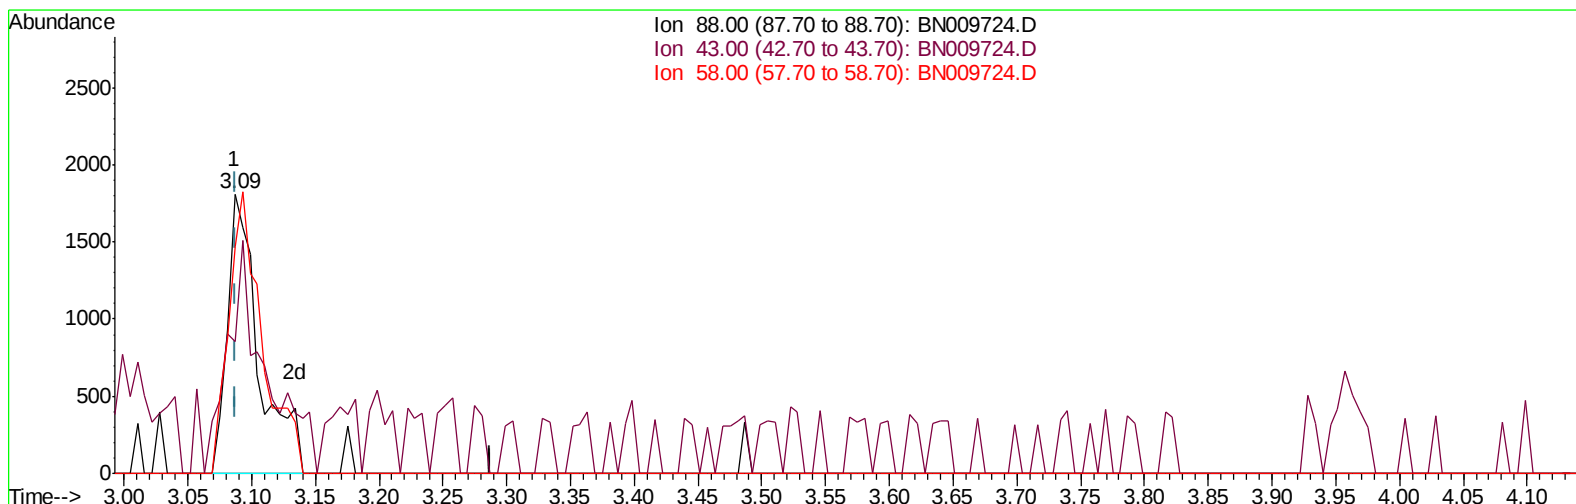

TIC: BN009724.D

(2) 1,4-Dioxane

3.087min (-0.000) 1.06ng/uL m

response 3092

Ion	Exp%	Act%
88.00	100	100
43.00	55.90	47.10
58.00	120.20	81.32#
0.00	0.00	0.00