

Data File : BN009725.D

Acq On : 14 Feb 2020 14:49

Operator : CG/JU

Sample : K5695-12

Misc : MDL-WATER-05

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Feb 17 00:52:36 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Feb 17 00:47:25 2020

Response via : Initial Calibration

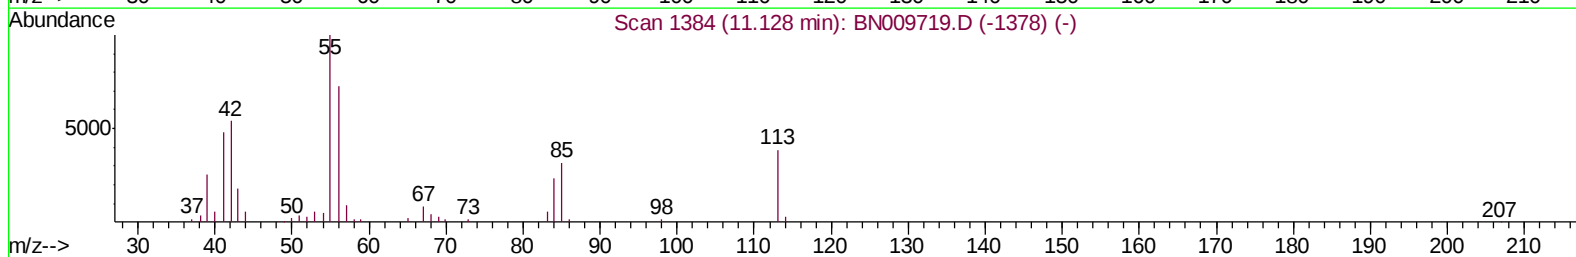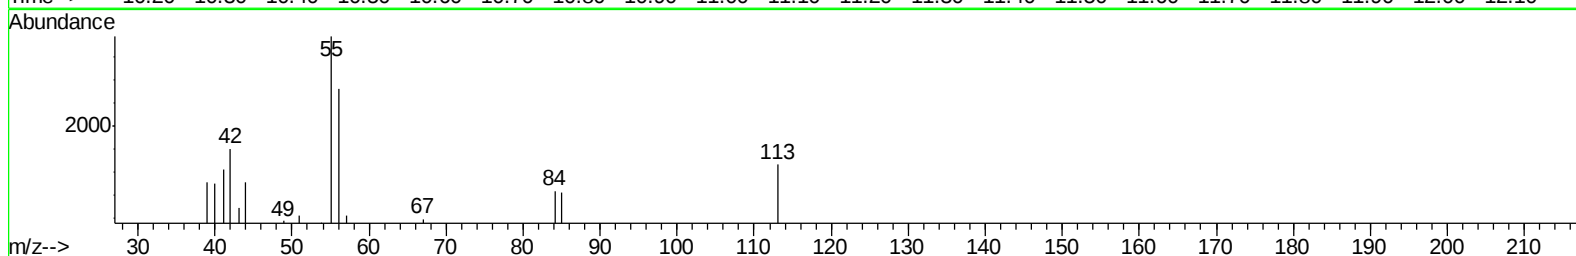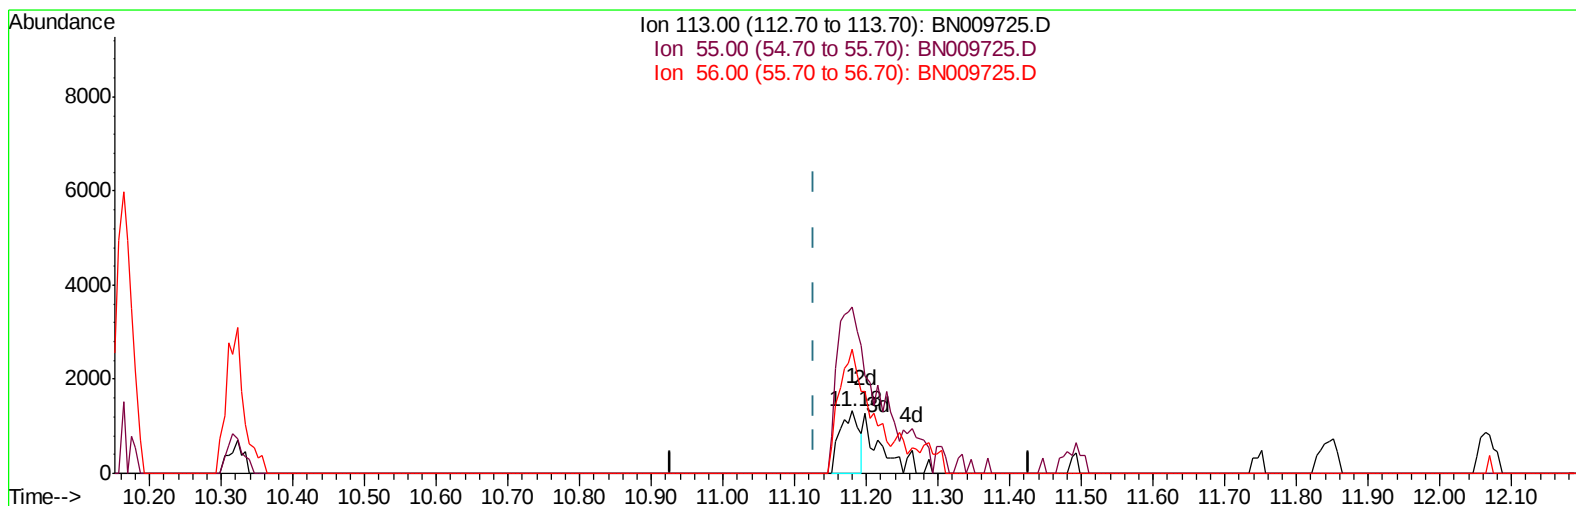

TIC: BN009725.D

(32) Caprolactam

11.181min (+0.053) 1.02ng/ul

response 2468

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	267.02
56.00	202.00	199.17
0.00	0.00	0.00