
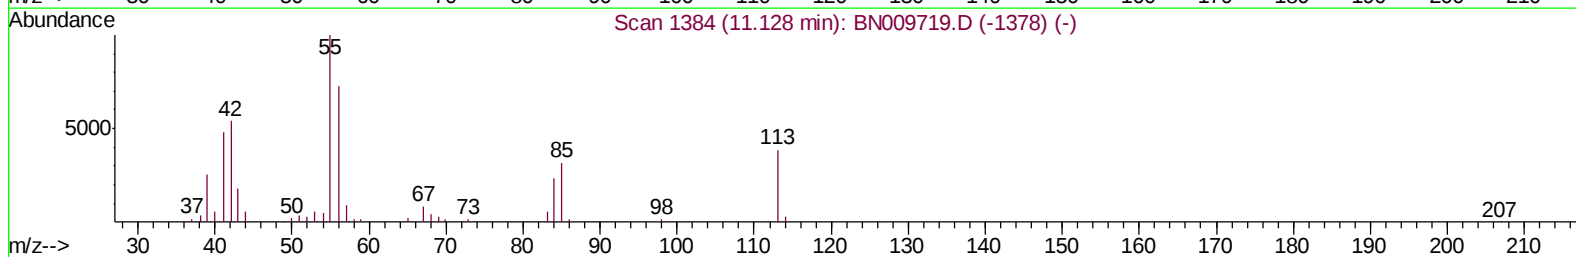
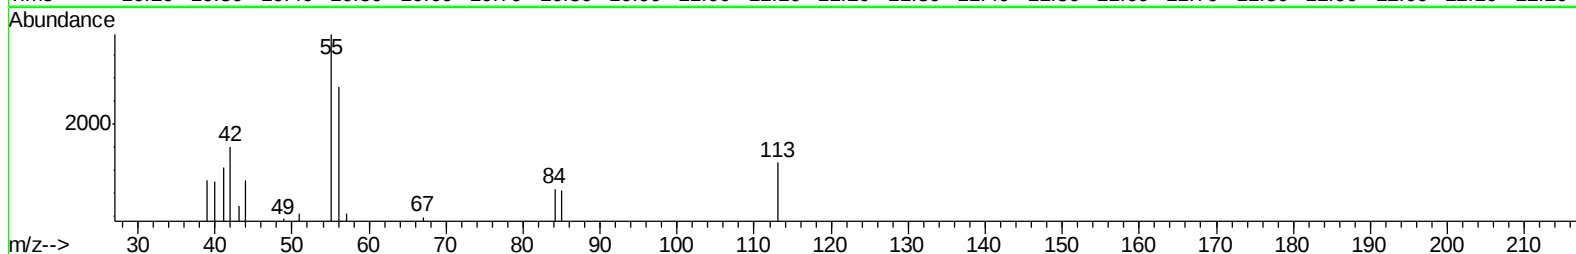


Data File : BN009725.D
Acq On : 14 Feb 2020 14:49
Operator : CG/JU
Sample : K5695-12
Misc : MDL-WATER-05
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Feb 17 00:52:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

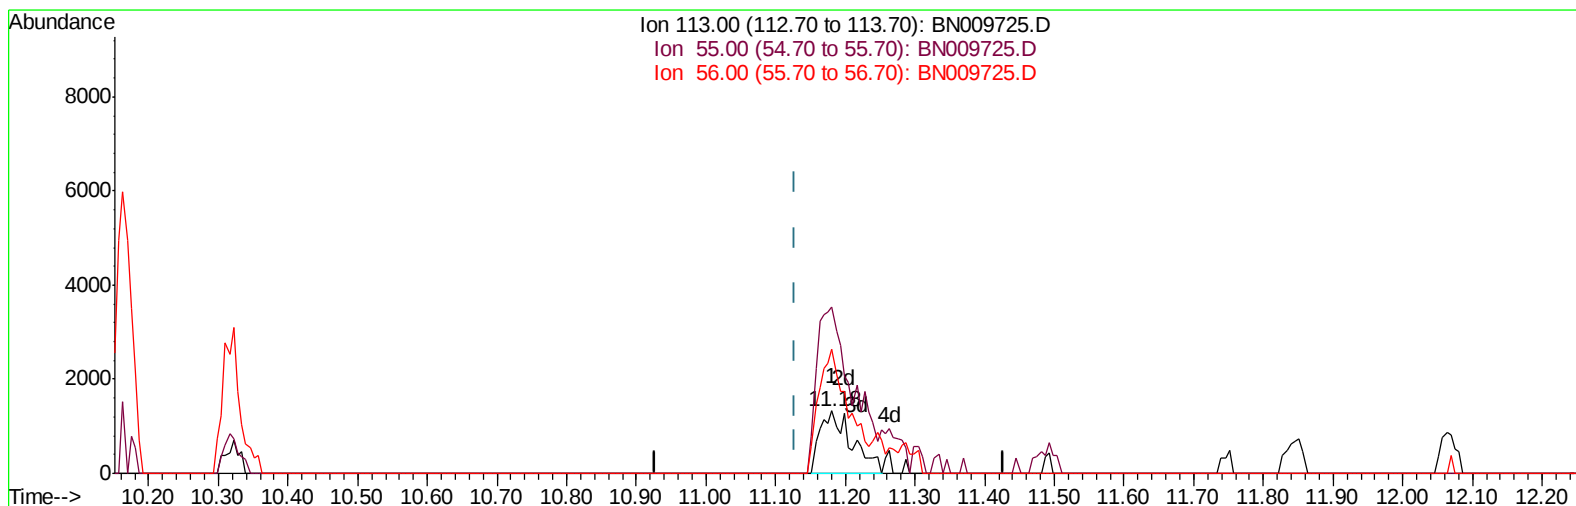

TIC: BN009725.D

(32) Caprolactam

11.181min (+0.053) 1.74ng/ul m

response 4207

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	267.02
56.00	202.00	199.17
0.00	0.00	0.00