
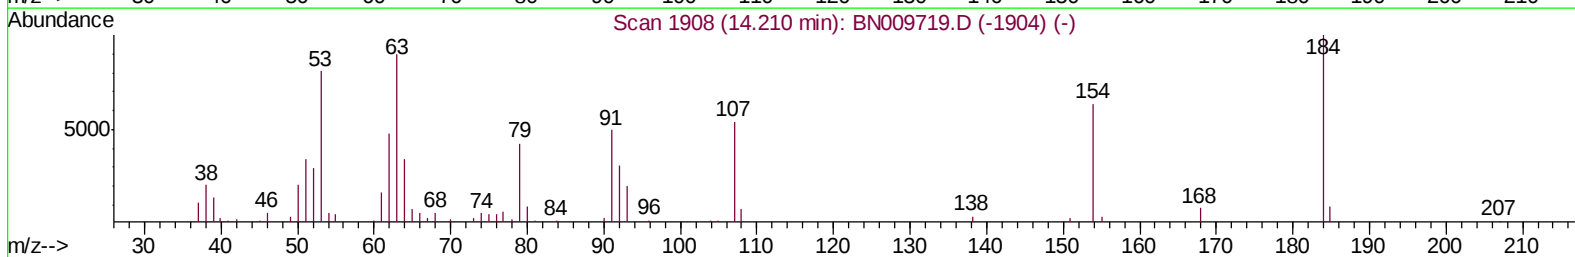
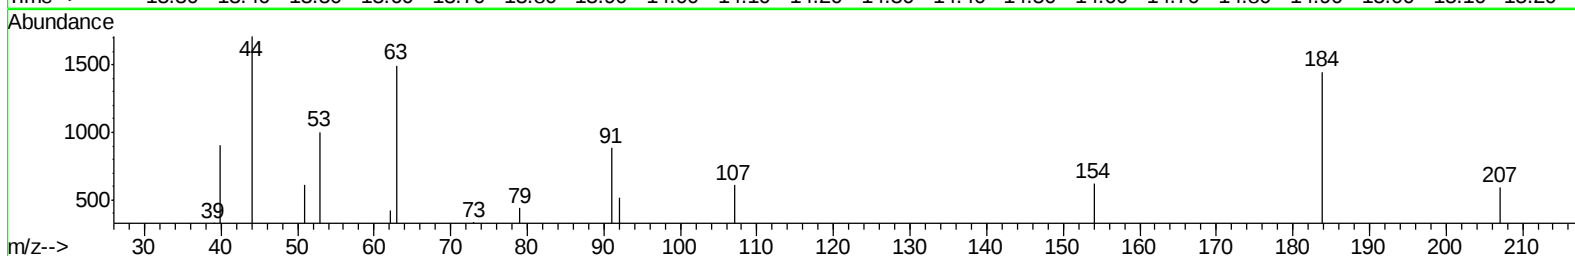


Data File : BN009725.D
Acq On : 14 Feb 2020 14:49
Operator : CG/JU
Sample : K5695-12
Misc : MDL-WATER-05
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Feb 17 00:52:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

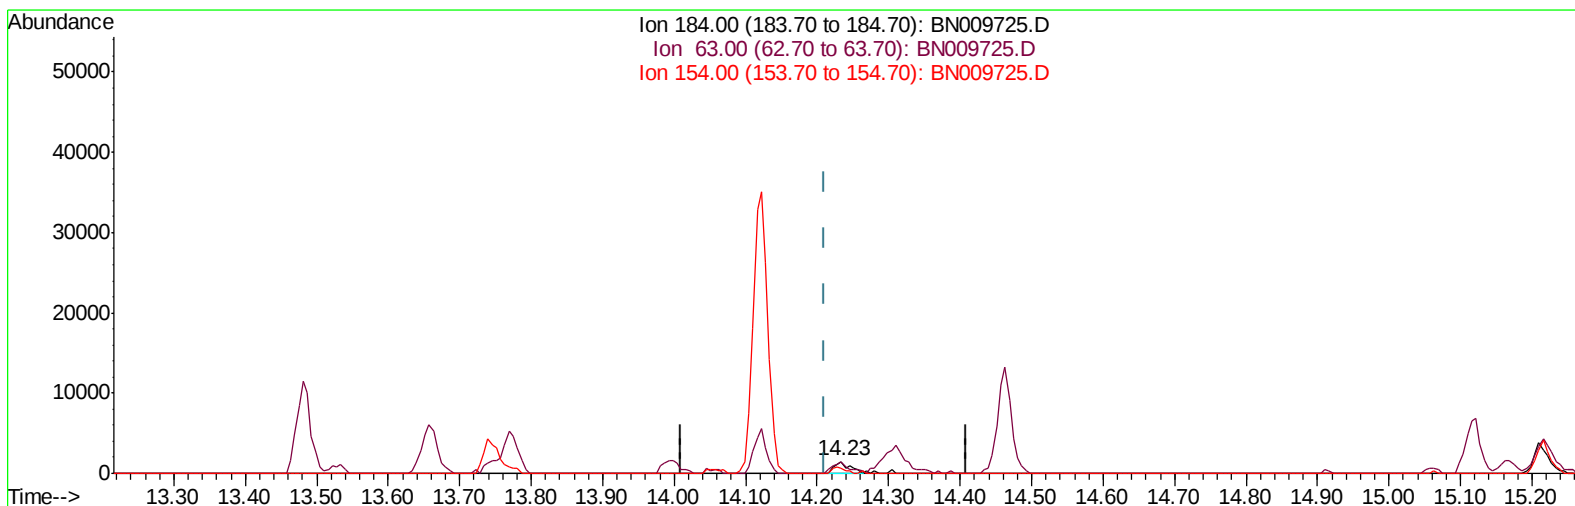

TIC: BN009725.D

(51) 2,4-Dinitrophenol

14.234min (+0.023) 0.88ng/ul m

response 2179

Ion	Exp%	Act%
184.00	100	100
63.00	103.80	103.24
154.00	68.60	42.86#
0.00	0.00	0.00